



ZOOM® View™ DISK

**Selected Episodes Report  
Induction 3**Device  
Tachy ModeTELIGEN  
Monitor + Therapy**Event V-1: 21 May 2010 10:01**

Event was Induced

**VF Event Onset**

Avg V Rate: 267 bpm

Detection: Rate Only

**At V-Detect**

Avg V Rate: 180 bpm

Rate Zone: VF

RhythmID Correlated: False

SRD Met: (False, Off)

ATP Timeout: False

**Attempt 1, 17 J V Shock**

Elapsed Time: 00:00:03

**Shock Information:**

Charge Time: 2.9 s

Lead Impedance: 61  $\Omega$ 

Lead Polarity: Initial

**At V-Detect**

Avg V Rate: 267 bpm

Rate Zone: VF

Stability: (25 ms, Off)

SRD Met: (False, Off)

ATP Timeout: False

**Attempt 2, 26 J V Shock**


Elapsed Time: 00:00:12




**Shock Information:**


Charge Time: 4.4 s

Lead Impedance: 61  $\Omega$ 


Lead Polarity: Initial

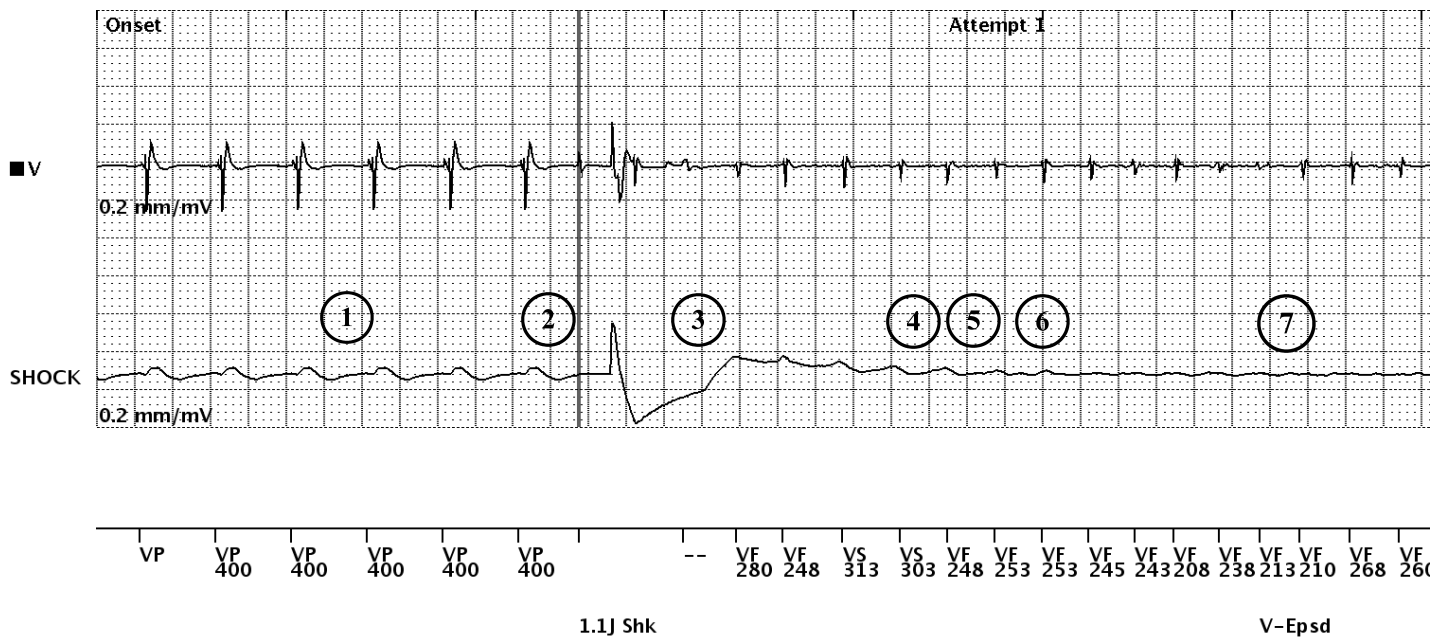**Event Ended 00:00:48**

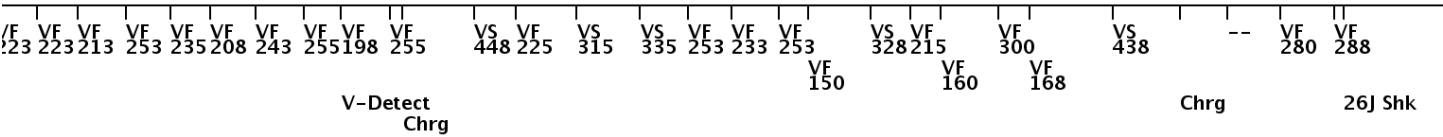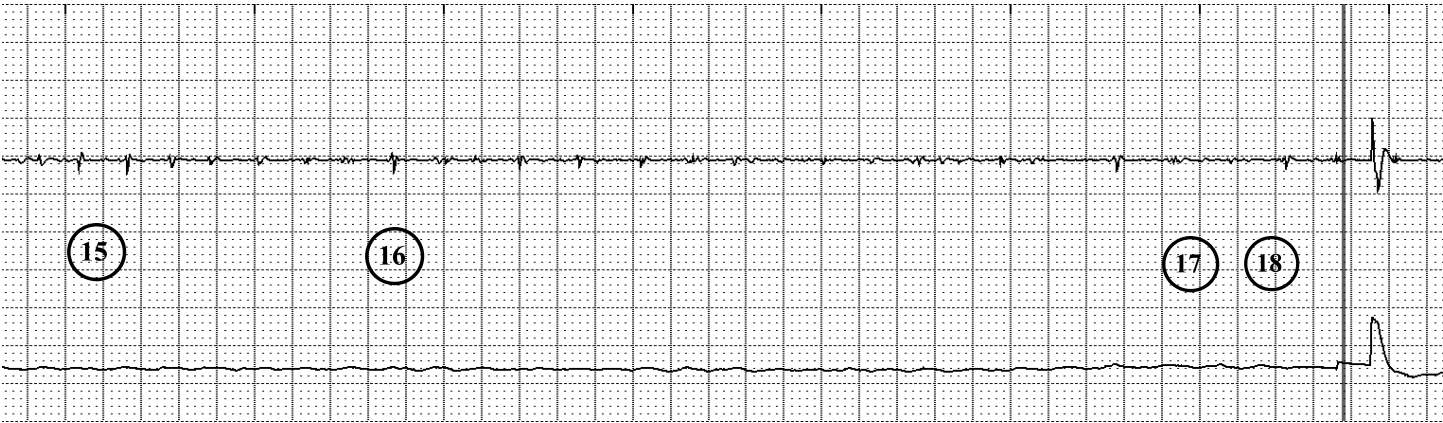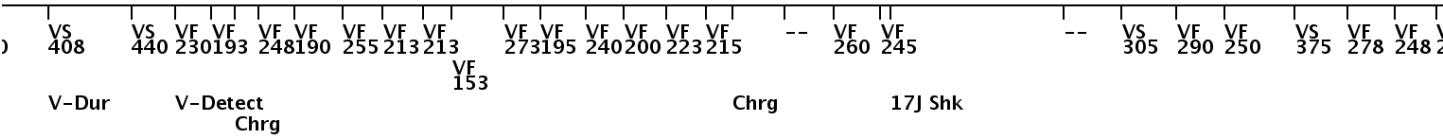

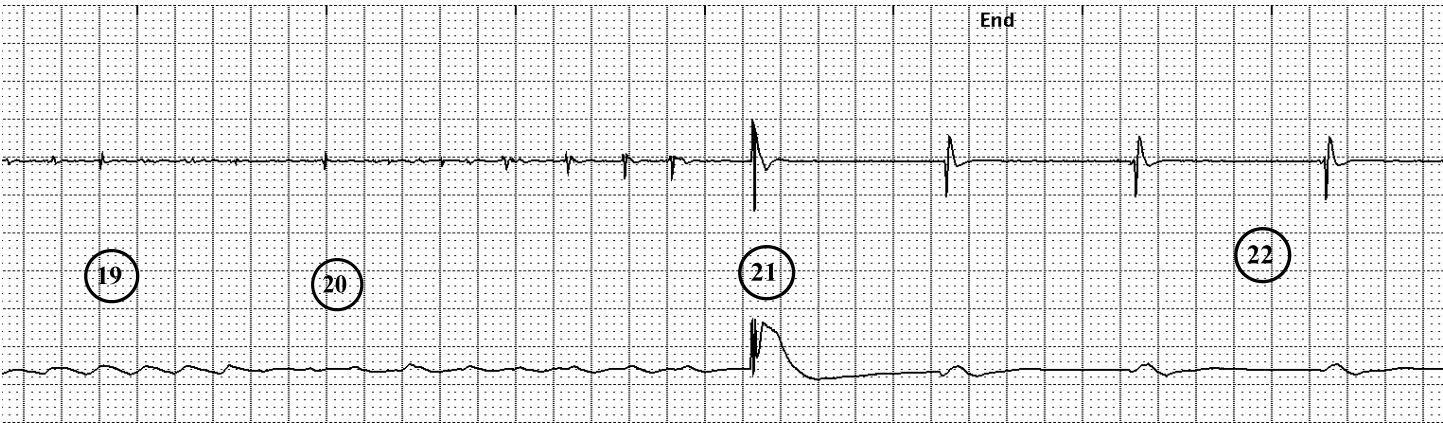

-- VS 488 VF 225 VS 453 VS 483 VF 155 VS 333 VS 303 VF 263 VS 420 VP 1000 VP 1000 VP 1000  
VF 150 VF 170

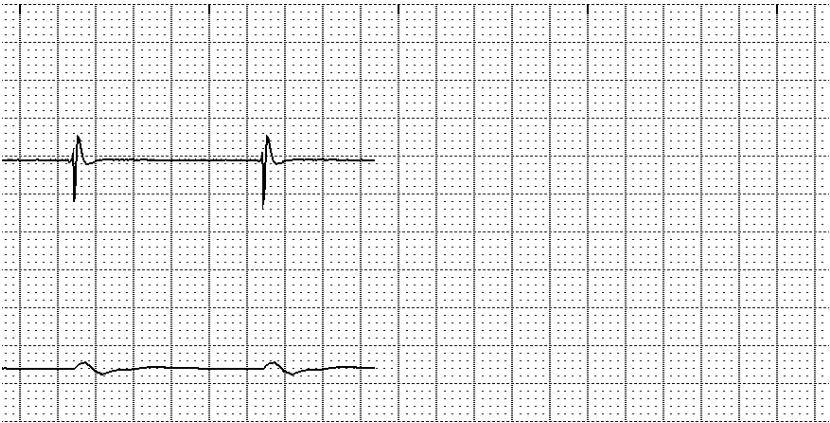

VP 1000 VP 1000

