



ZOOM® View™ DISK
Selected Episodes Report

Device COGNIS
Tachy Mode Monitor + Therapy

Event V-65: 13 Sep 2012 13:11

VT Event Onset

Avg A Rate: 105 bpm
Avg V Rate: 141 bpm
Detection: Onset/Stability
Onset: Percent

At V-Detect

Avg A Rate: 82 bpm
Avg V Rate: 131 bpm
Rate Zone: VT
Stability: 384 ms
V>A Rate: True
AFib: False
SRD Met: (False, Off)
ATP Timeout: False
Onset Intvl: (355 ms, Off)
Onset %: 35 %


Attempt 1, Scan V ATP



Elapsed Time: 00:00:29


ATP Information:


Number of Bursts: 1

Event Ended 00:00:43

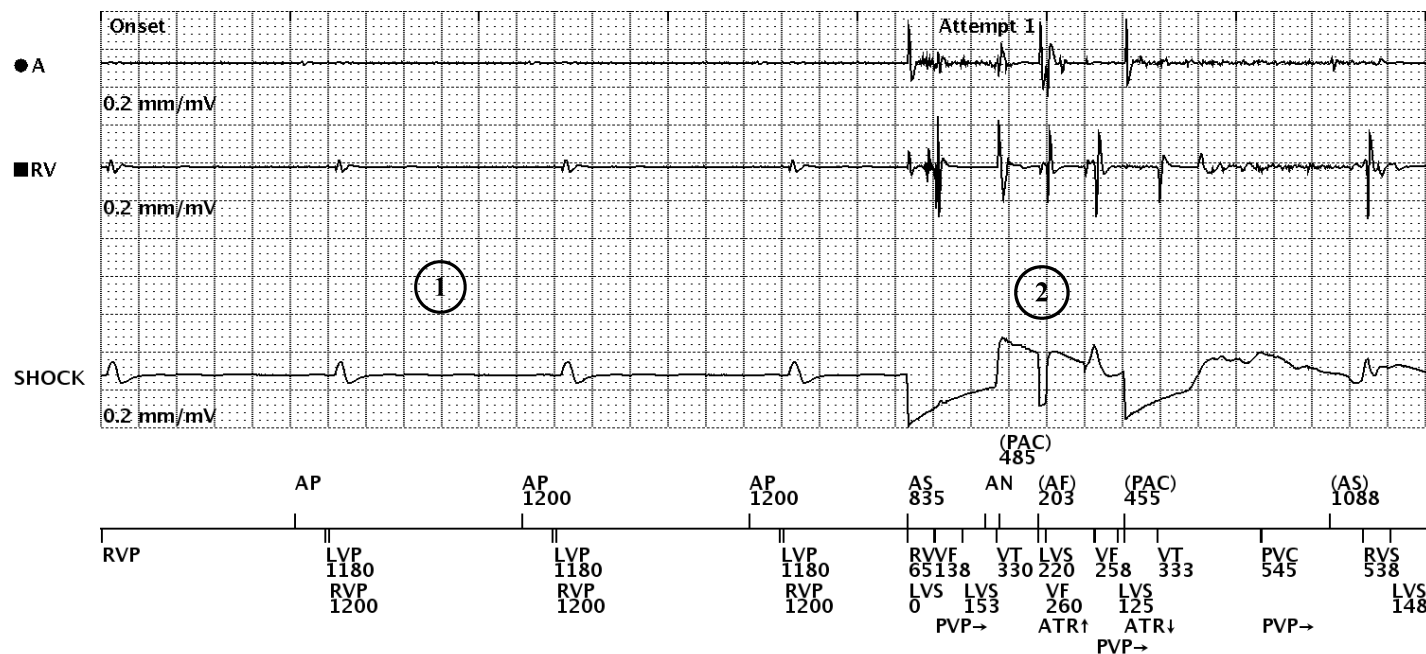


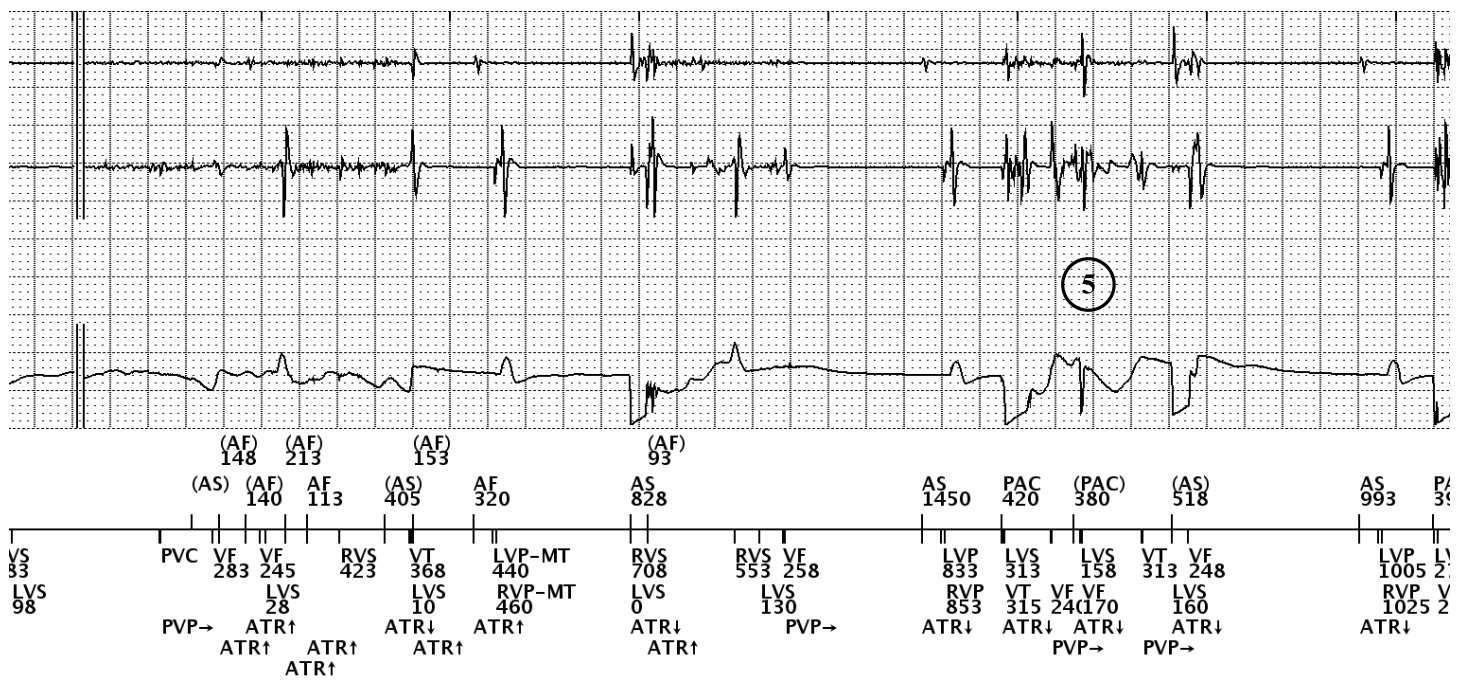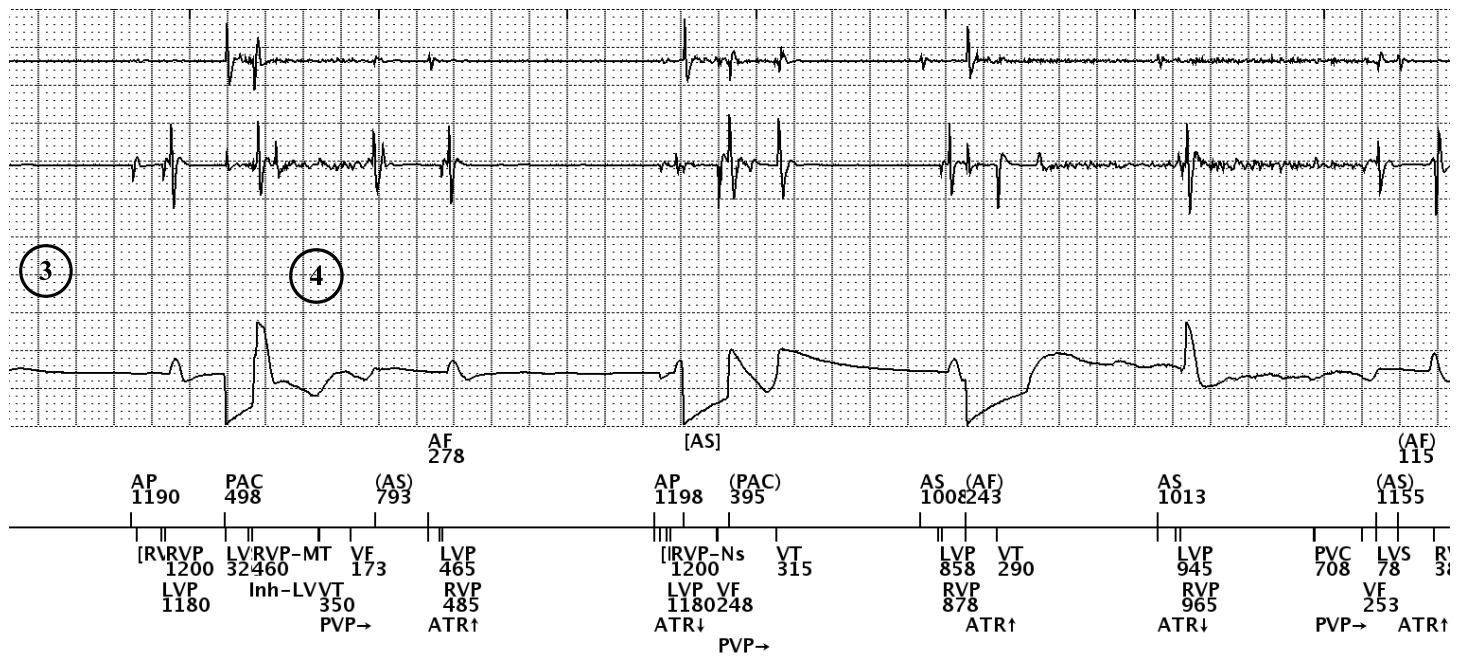


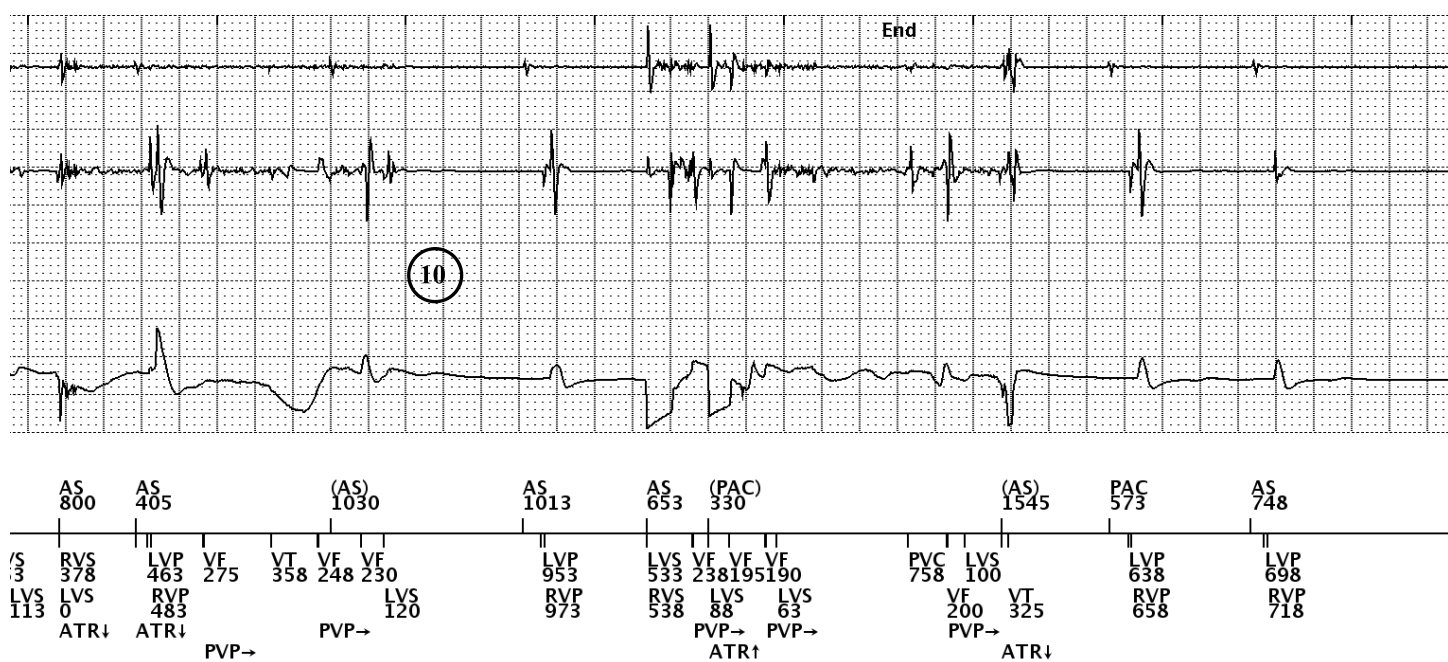

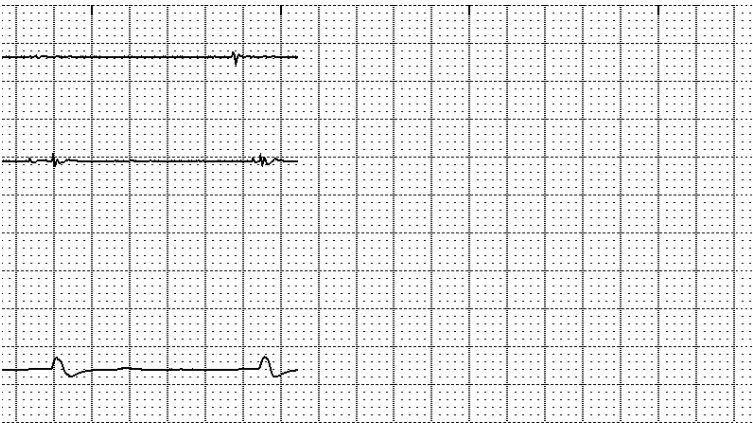

- A Sense
- V Sense
- A Pace
- V Pace
- ↑ > A Range
- ↑ > V Range
- ↓ < A Range
- ↓ < V Range

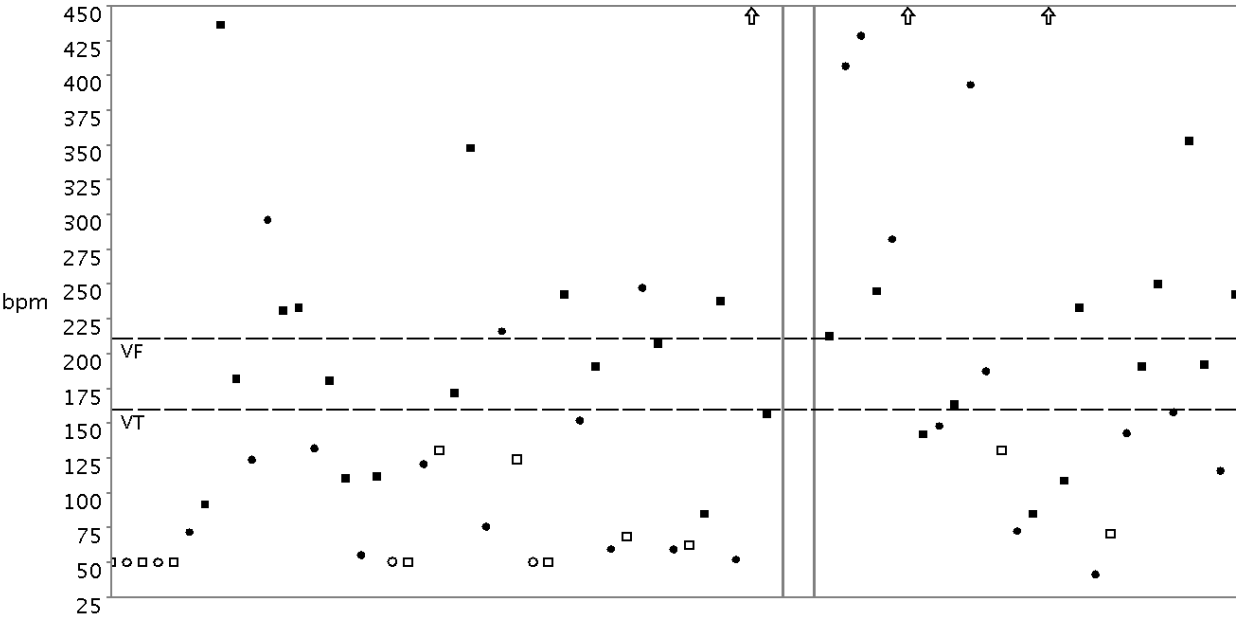

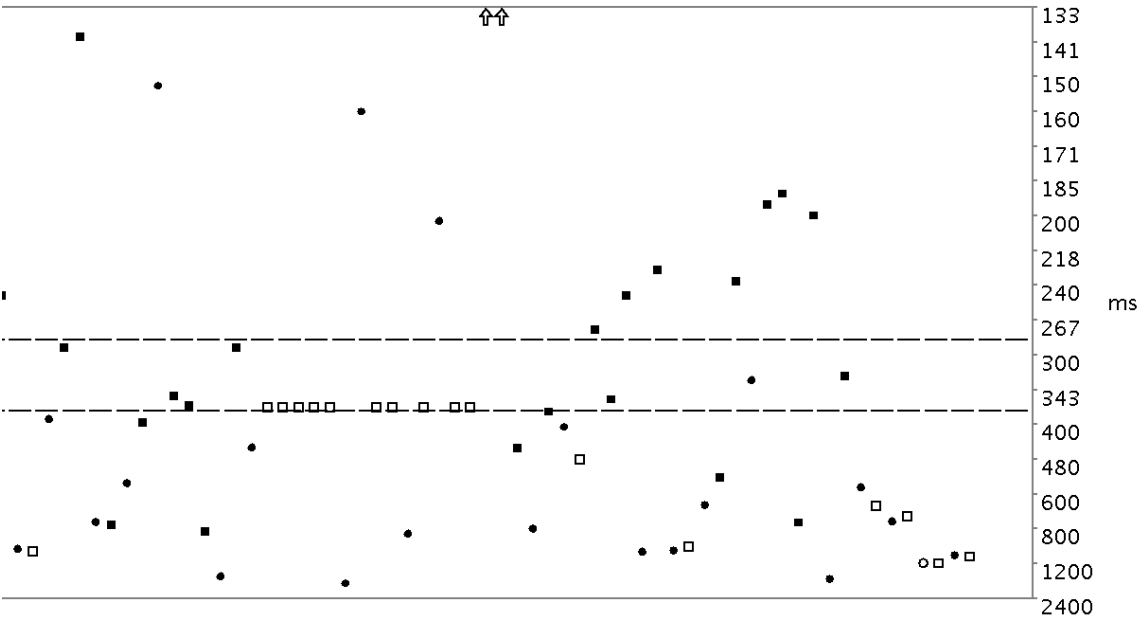



ZOOM® View™ DISK
Selected Episodes Report

Device COGNIS
Tachy Mode Monitor + Therapy

Event V-70: 13 Sep 2012 13:14

VF Event Onset

Avg A Rate: 124 bpm
Avg V Rate: 178 bpm
Detection: Onset/Stability
Onset: Percent

At V-Detect

Avg A Rate: 75 bpm
Avg V Rate: 115 bpm
Rate Zone: VF
Stability: (321 ms, Off)
V>A Rate: (True, Off)
AFib: (False, Off)
SRD Met: (False, Off)
ATP Timeout: False
Onset Intvl: (331 ms, Off)
Onset %: 50 %

Attempt 1, Non Therapy V

Elapsed Time: 00:00:04

Attempt Information:

No therapy delivered, Tachy therapy mode is not programmed to Monitor+Therapy.

Event Ended 00:00:14

