

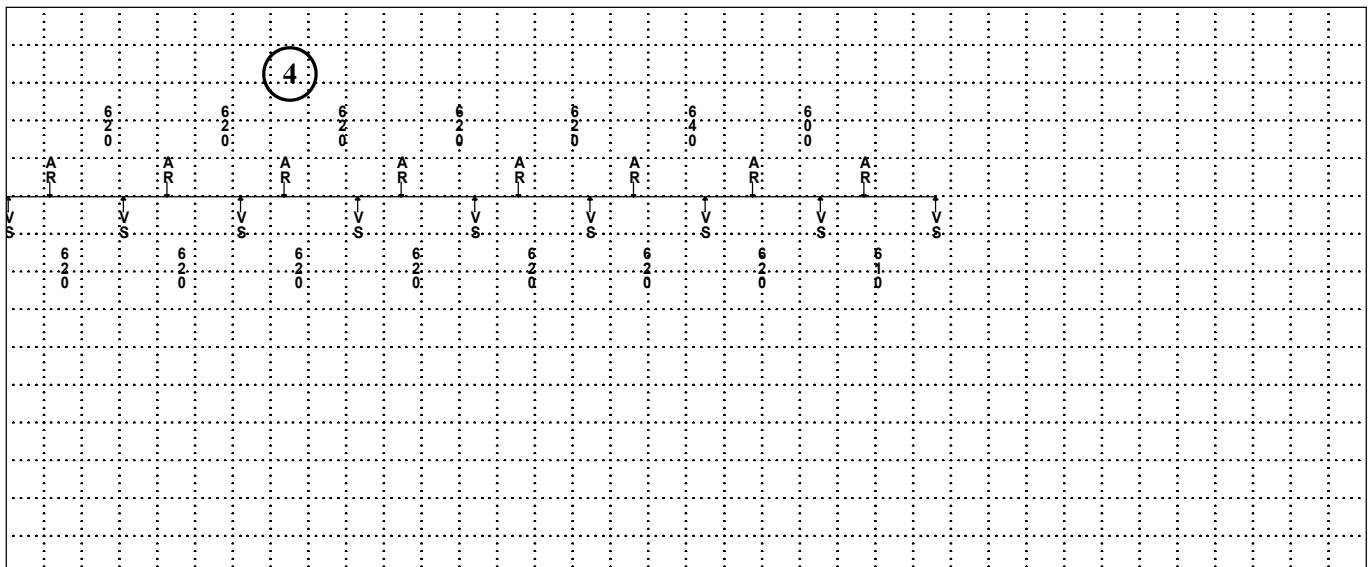
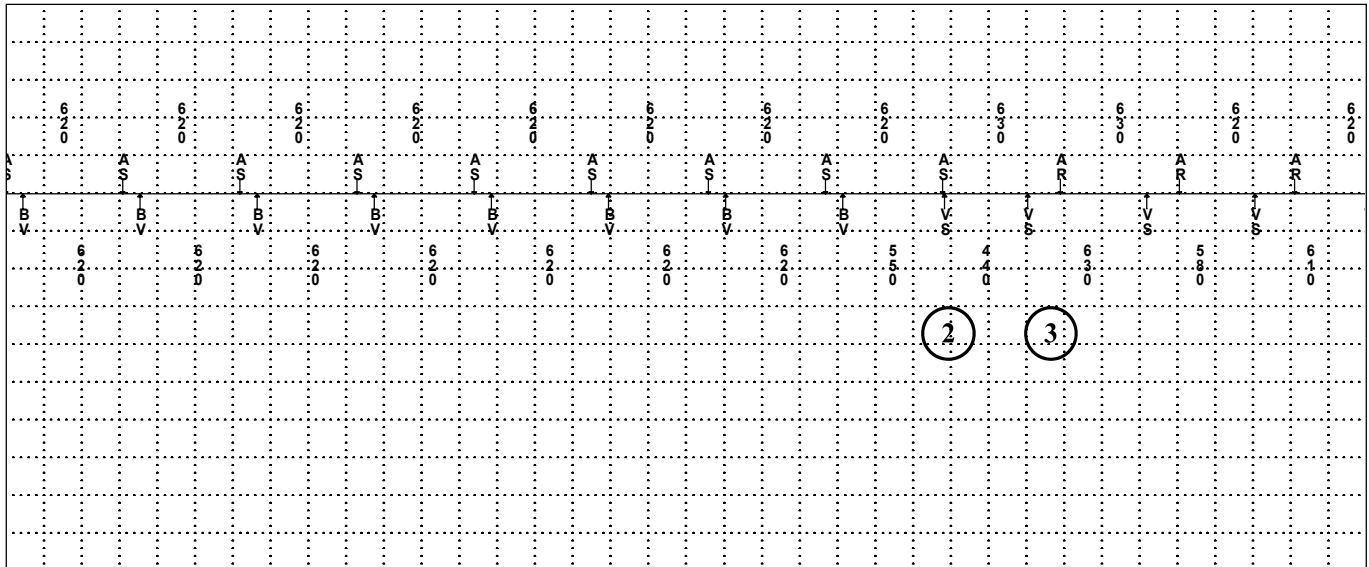
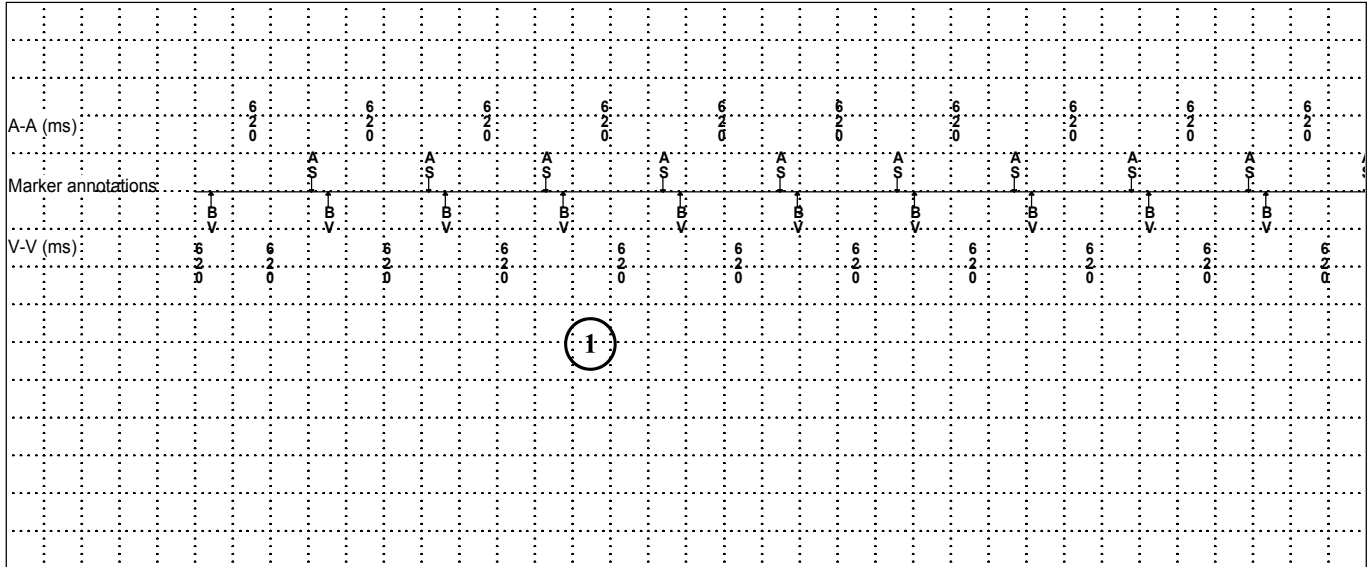
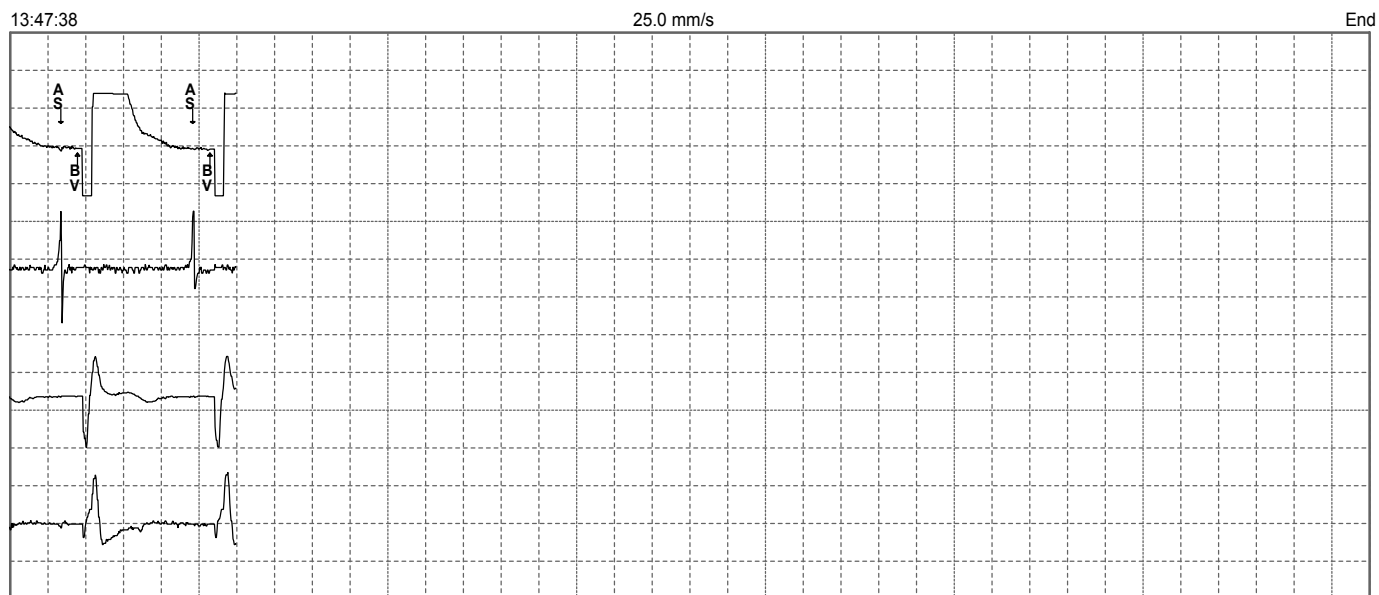


Monitored Ventricular Episode # 1194

Device: Protecta XT CRT-D D354TRG

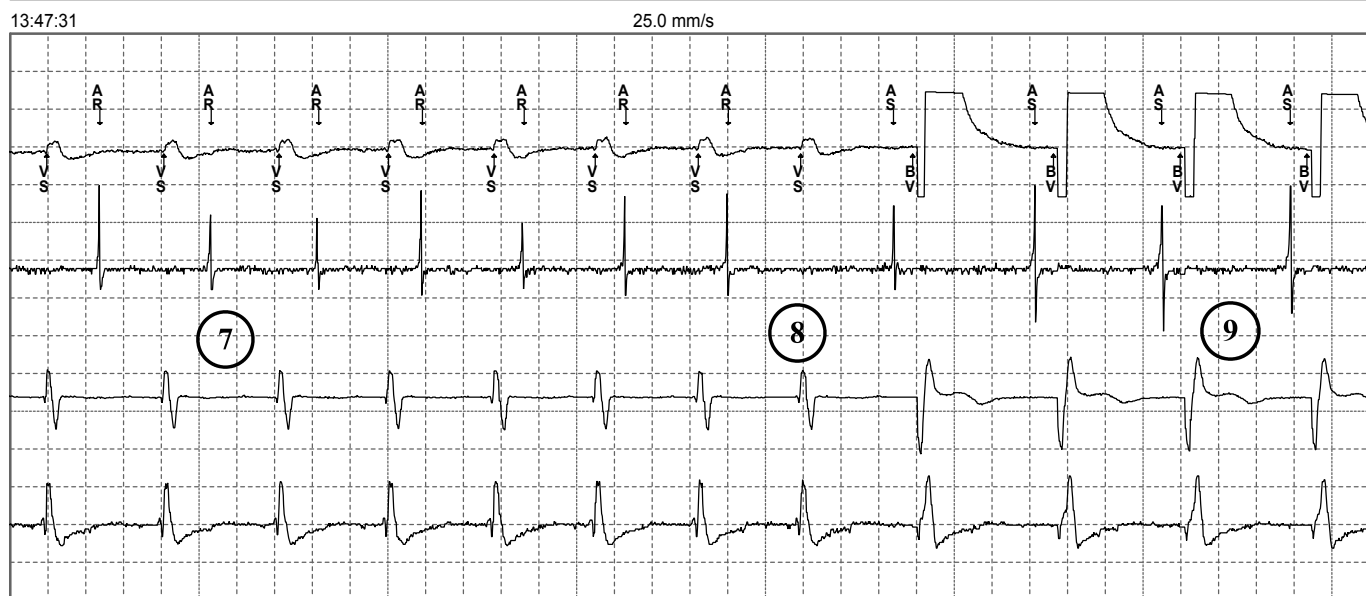

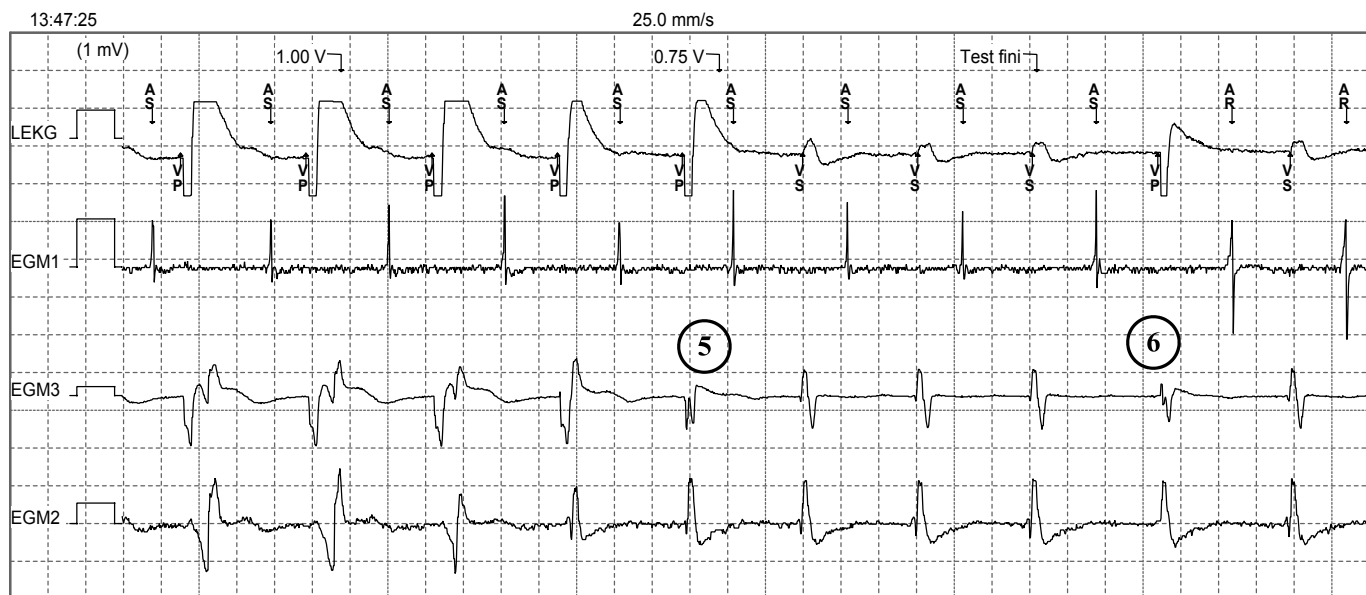

Device : Protecta XT CRT-D D354TRG

