

Non-sustained VT Episode #53 Serial  
Number:

Device : Protecta XT CRT-D D354TRG

Date of visit : 11-Jun-2013 10:34:22

Patient :

ID :

Physician :

Type	ATP Seq	Shocks	Success	ID#	Date	Time hh:mm	Duration hh:mm:ss	Avg bpm A/V	Max bpm A/V	Activity at Onset
VT-NS				53	28-Apr-2013	09:12	:01	110/200		Rest


• V-V

□ A-A

VF = 222 ms

VT = 171 min<sup>-1</sup>

Term

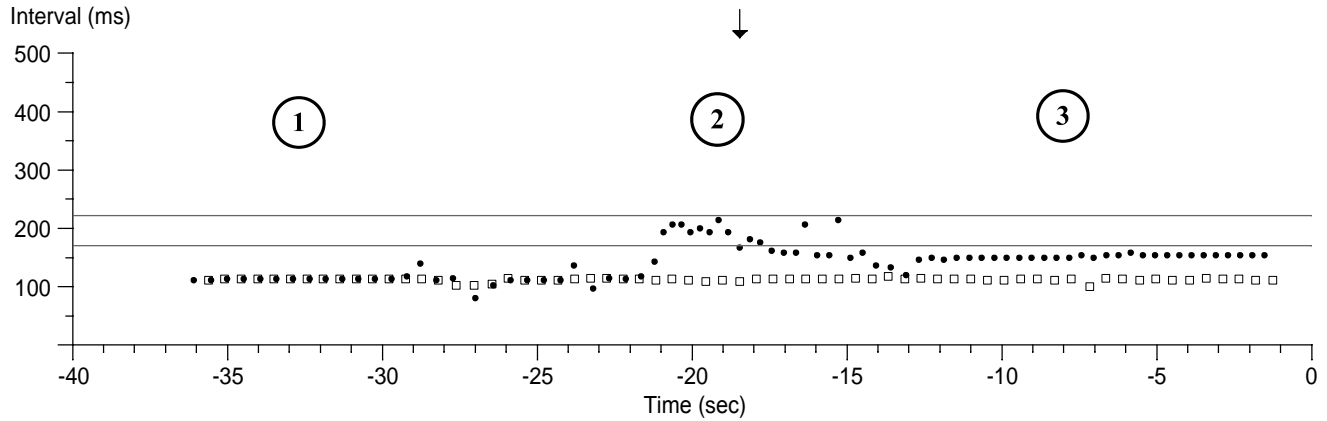

# Non-sustained VT Episode #53

Device: **Protecta XT CRT-D D354TRG**




Serial Number:

Date of Visit: **12-Jun-2013 13:35:04**

Patient: -

ID:

Episode #53 Chart speed: 25.0 mm/sec

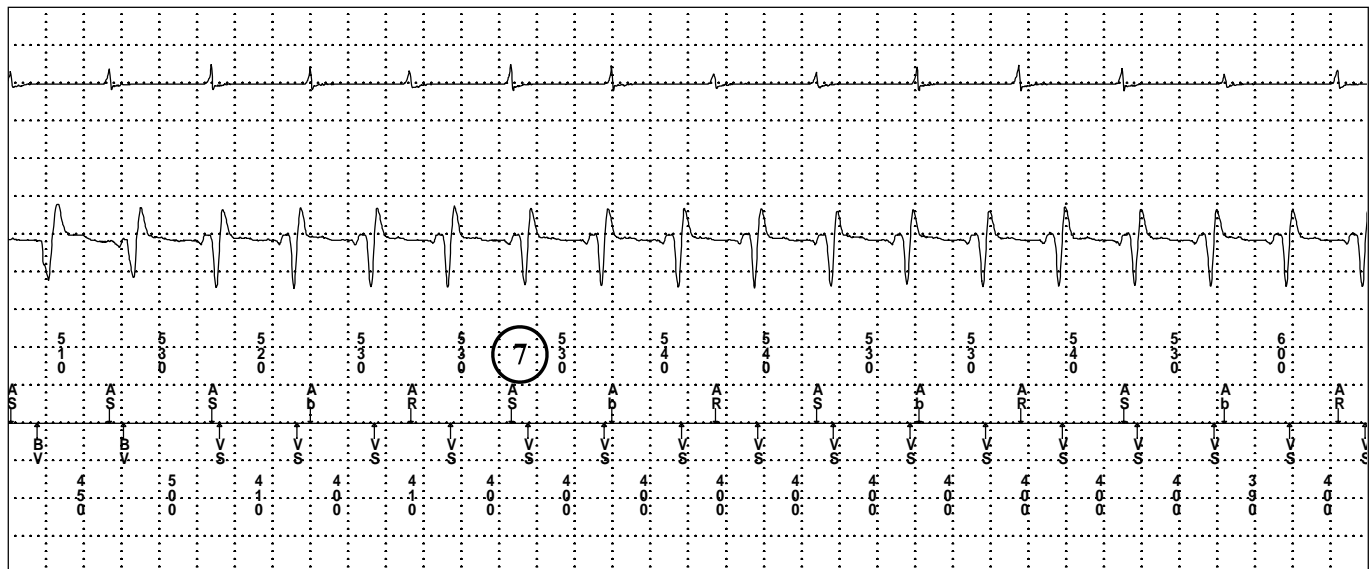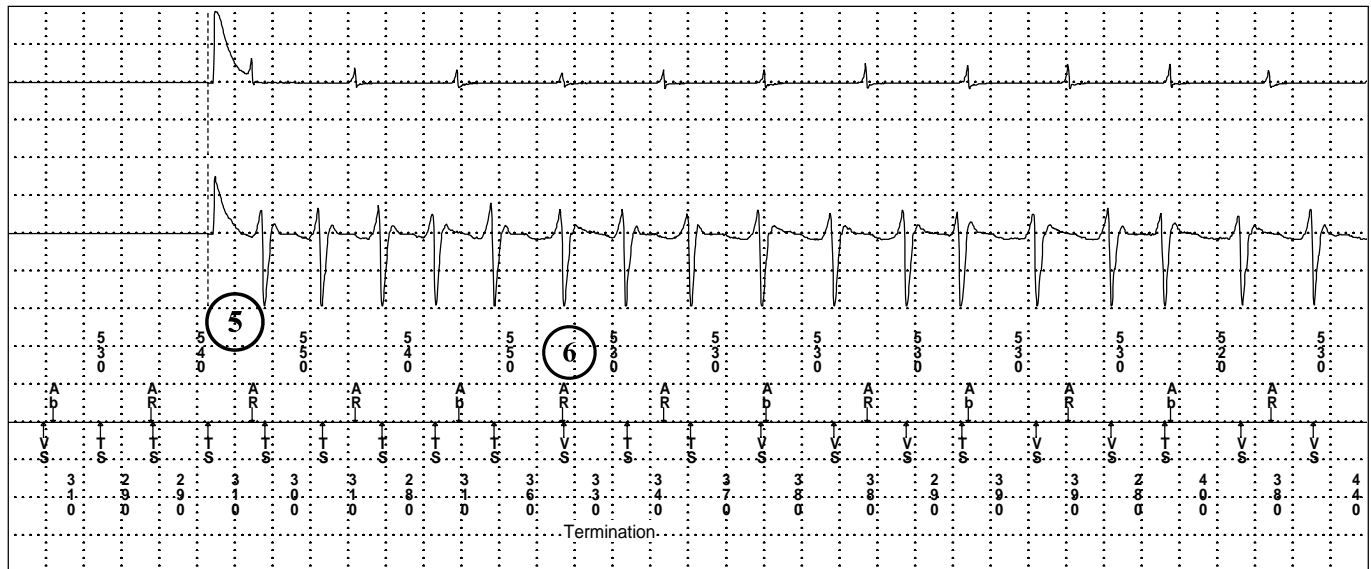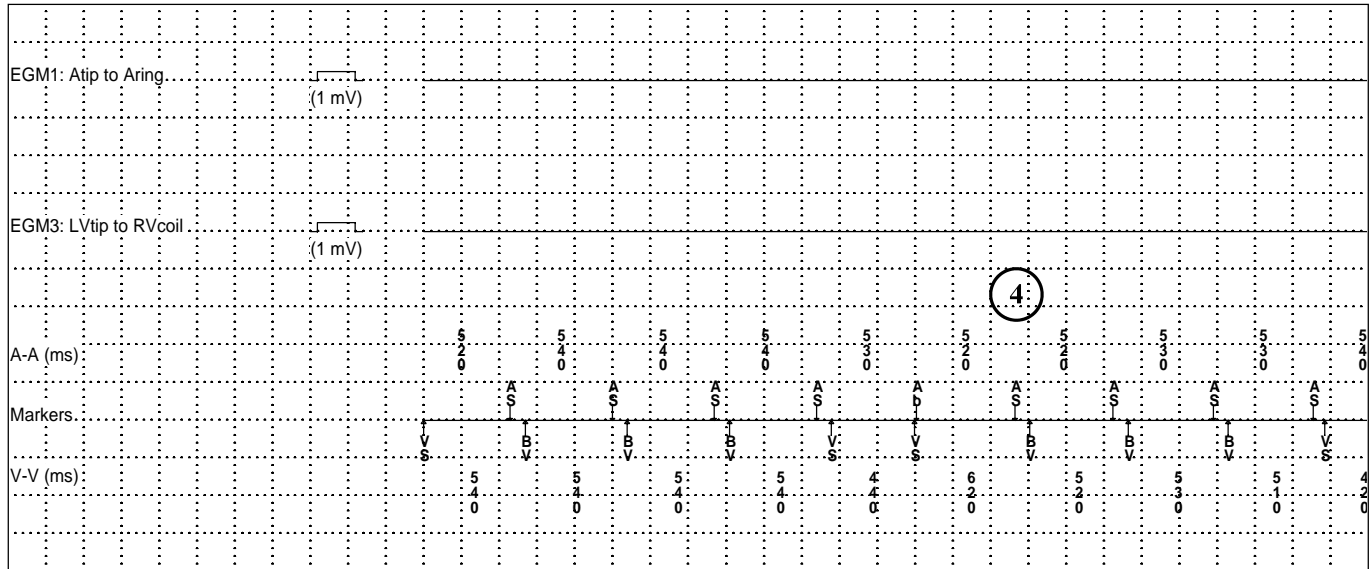

# Non-sustained VT Episode #53

Device: **Protecta XT CRT-D D354TRG**

Serial Number:

Date of Visit: **12-Jun-2013 13:35:04**

Patient:

ID:

**Episode #53** Chart speed: 25.0 mm/sec

