



Date of Birth:
Device:
Clinic:
Search Tags:
Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **26 Oct 2015 04:02 CET**
Last Office Interrogation: **20 Jul 2015**
Implant Date: **22 Oct 2014**
Patient Group:

V-25: 21 Dec 2014 04:11, VT-1, A Rate: 48 min⁻¹, V Rate: 178 min⁻¹

Detail

VT-1 Event Onset

Avg A Rate	48 min ⁻¹
Avg V Rate	178 min ⁻¹
Detection	Onset/Stability
Onset	Percent
Template	N/R

At V-Detect

Avg A Rate	39 min ⁻¹
Avg V Rate	175 min ⁻¹
Rate Zone	VT
Stability	13 ms
V>A Rate	True
AFib	False
RhythmMatch™	N/R
SRD Met	(False, Off)
ATP Timeout	False
Onset Intvl	(365 ms, Off)
Onset %	39 %


Attempt 1, Burst V ATP

Elapsed Time	00:00:04
ATP Information	
Number of Bursts	1

Event Ended

00:00:18


EGM displayed at 25mm per second

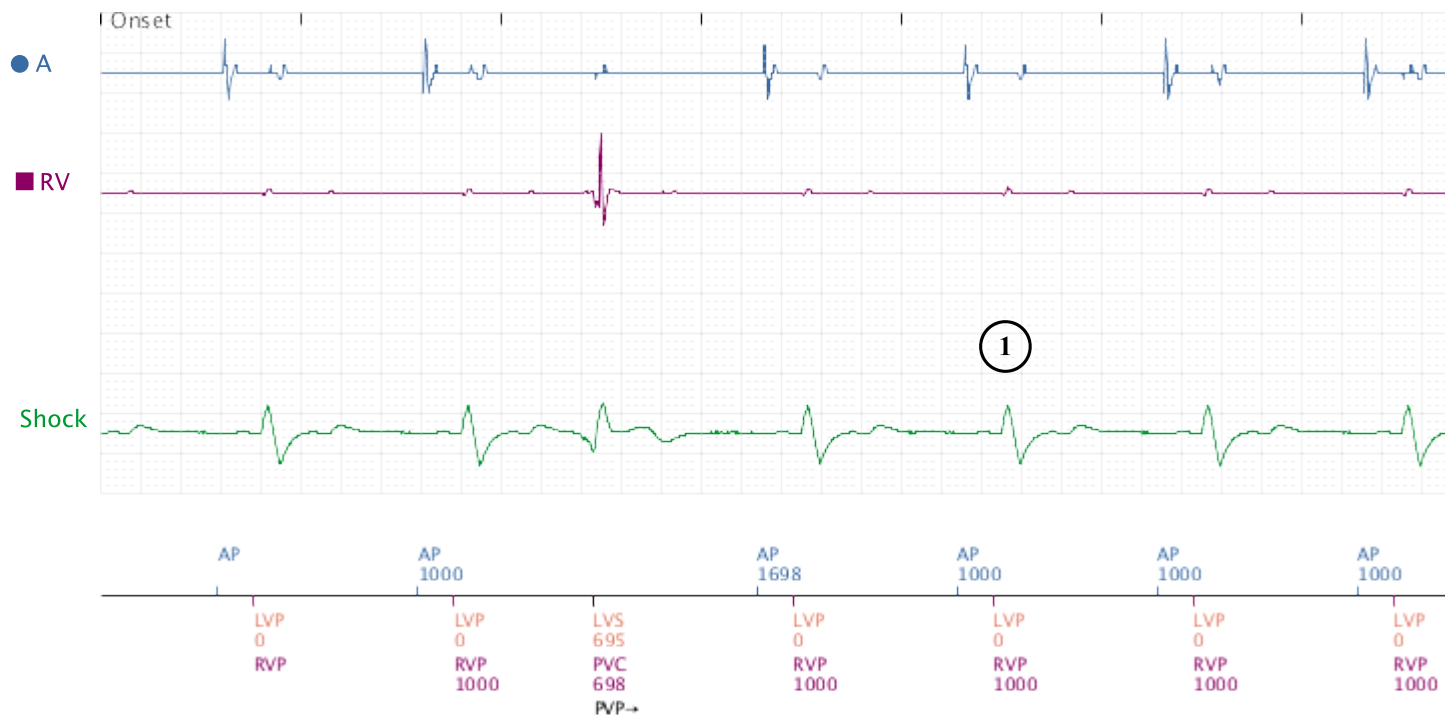



2

LVS	VT-1	VT-1	VT-1	VT	VT	VT	VT-1	VT	VT	VT	VT	VT	VT-1	VT-1	VT	VT-1	VT	V
0	448	398	365	330	313	343	355	345	335	335	330	338	360	363	353	363	330	3
PVC	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	
635	53	58	60	55	58	60	58	60	58	63	58	60	63	60	58	58	58	
PVP→		PVP→		PVP→		PVP→		V-Epsd										
								Sudden										

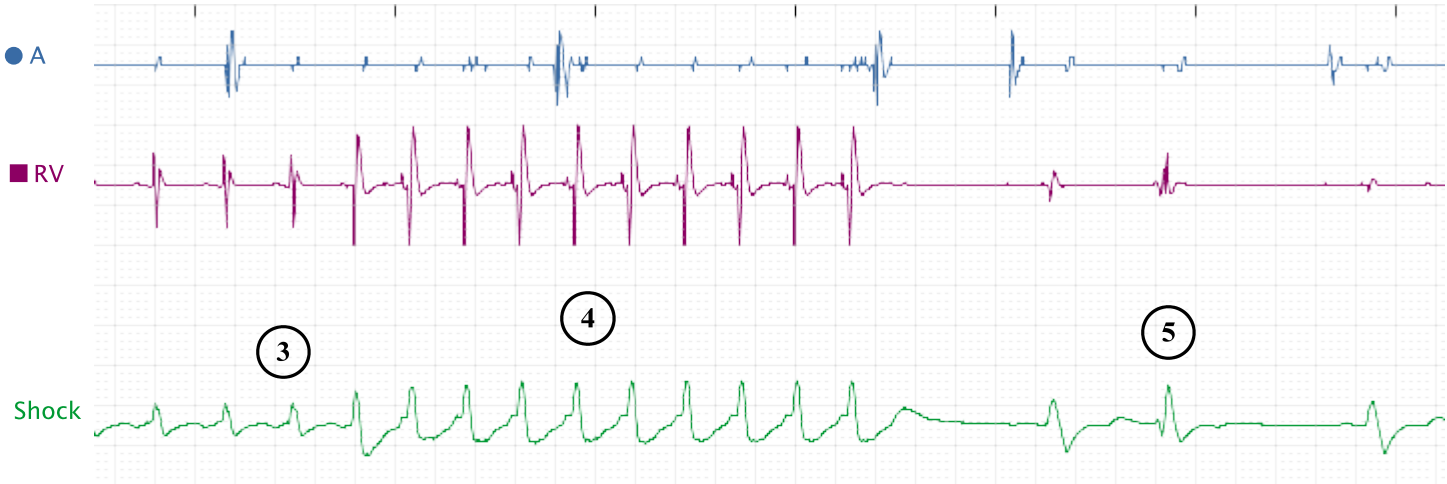

3

4

5

T	VT	VT	VT	LVP	LVP	LVP	LVP	LVP	LVP	LVP	LVP	LVP	LVP	LVP	AP	LVP	PVC	LVP
45	345	350	335	0	0	0	0	0	0	0	0	0	0	0	640	0	593	0
LVS	LVS	LVS		RVP	RVP	RVP	RVP	RVP	RVP	RVP	RVP	RVP	RVP	RVP		RVP	LVS	RVP
60	58	58		275	275	275	275	275	275	275	275	275	275	275		1000	10	1000
			V-Dur											PVP→			PVP→	
			V-Detect															
			Sth															
			V>A															



↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	○ A Pace

