

Episode: VT-2 (190 bpm / 315 ms)

VT/VF Episode 13 of 25

Page 1 of 3

Duration 00:14 (M:S) No Alerts
Detection Criteria 190 - 221 bpm

Therapy	Results
1) ATP	1) Below Rate Detection (CL 730 ms)

ATP Therapy Details

VT-2 ATP Therapy

Successful BCL 264 ms
Therapy 1
Burst 1 264, 264, 264, 264, 264, 264, 264, 264 ms

Diagnosis Summary

	Diagnosis
	VT-2
Time to Diagnosis	7.25 sec
Rate (CL)	190 bpm (315 ms)
Zone	VT-2
Rate Branch Classification	VT (V > A) Rate Branch

SVT Criteria Statistics

SVT Diagnoses during this episode 0

DeFT Response™ Settings (Shock Waveform)

			1st Phase	2nd Phase
Waveform	Biphasic	VF Shocks (Defib)	65 %	65 %
Waveform Mode	Tilt	VT Shocks (CVRT)	Same as Defib	Same as Defib
Shock Configuration	RV to Can			
RV Polarity	Anode(+)			
Defib Max Sensitivity	0.3 mV			

Episode: VT-2 (190 bpm / 315 ms)

VT/VF Episode 13 of 25




Page 2 of 3

1: A Sense Amp AutoGain (1.8 mm/mV)

3: Markers

2: V Sense Amp AutoGain (0.4 mm/mV)

Sweep Speed: 25 mm/s

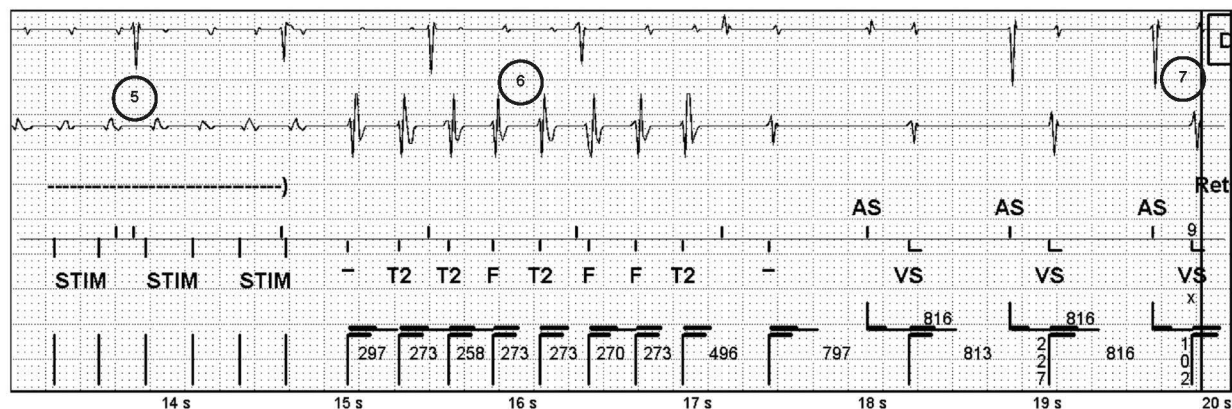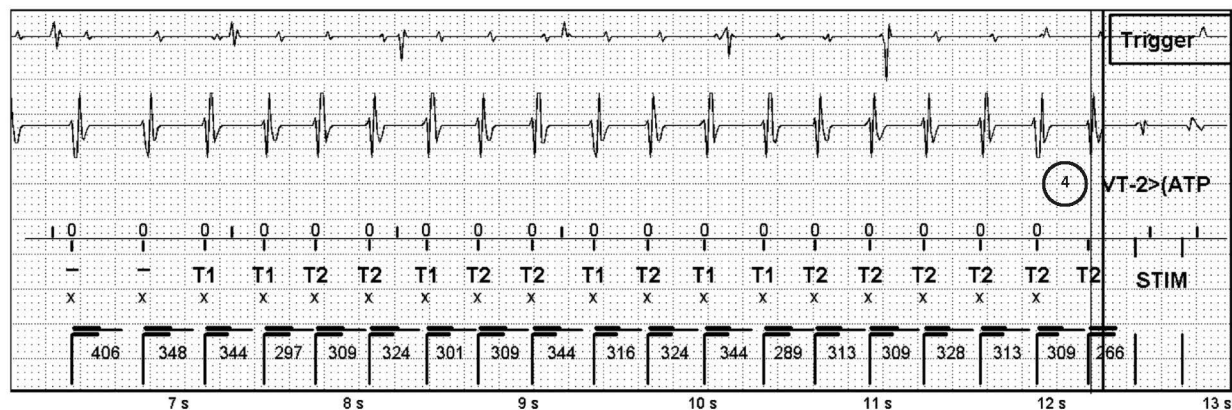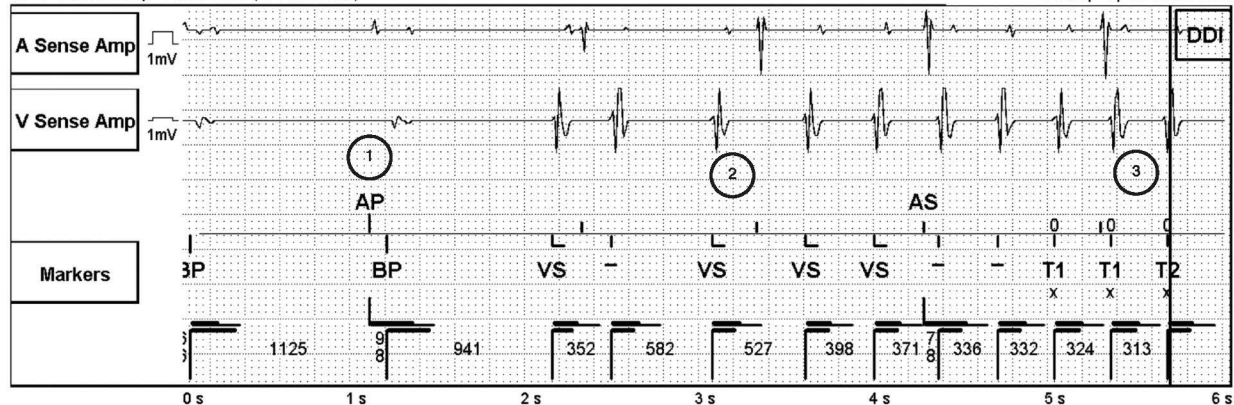

Episode: VT-2 (190 bpm / 315 ms) (Continued)

VT/VF Episode 13 of 25

Page 3 of 3

1: A Sense Amp AutoGain (1.8 mm/mV)

3: Markers

2: V Sense Amp AutoGain (0.4 mm/mV)

Sweep Speed: 25 mm/s

