



Episode: SVT (144 bpm / 415 ms)

VT/VF Episode 42 of 63

Page 1 of 3

Duration 00:20 (M:S) No Alerts
Detection Criteria 142 - 213 bpm

Therapy

No therapies were delivered

Results

Diagnosis Summary

	Diagnosis
	SVT
Time to Diagnosis	7.75 sec
Rate (CL)	144 bpm (415 ms)
Zone	VT-1
VT Diagnosis Criteria	All
Rate Branch Classification	AF/AFL (V < A) Rate Branch

Morphology

On, ≥ 60% is a match, ≥ 5 matches indicate SVT
Min Match Score 98%
Max Non-Match Score n/a
No. Template Matches 8 of 8 **(SVT Indicated)**

Interval Stability

On, ≥ 50 ms indicates SVT (AVA Delta Passive, < 60 ms indicates SVT)
Stability Delta 115 ms **(SVT Indicated)**

SVT Criteria Statistics

SVT Diagnoses during this episode 2

Measured SVT Discriminator values for Episode

Min Match Score	98 %	Min/Max Stability Delta	115 ms /135 ms
Max Non-Match Score	0 %	Template Used	2 Dec 2009 11:25

DeFT Response™ Settings (Shock Waveform)

Waveform	Biphasic	VF Shocks (Defib)	1st Phase	2nd Phase
Waveform Mode	Tilt	VT Shocks (CVRT)	65 %	65 %
Shock Configuration	RV to SVC & Can		Same as Defib	Same as Defib
RV Polarity	Anode(+)			
Defib Max Sensitivity	0.3 mV			



Episode: SVT (144 bpm / 415 ms)

VT/VF Episode 42 of 63




Page 2 of 3

1: A Sense Amp AutoGain (1.4 mm/mV)

3: Markers

2: V Sense Amp AutoGain (0.4 mm/mV)

Sweep Speed: 25 mm/s

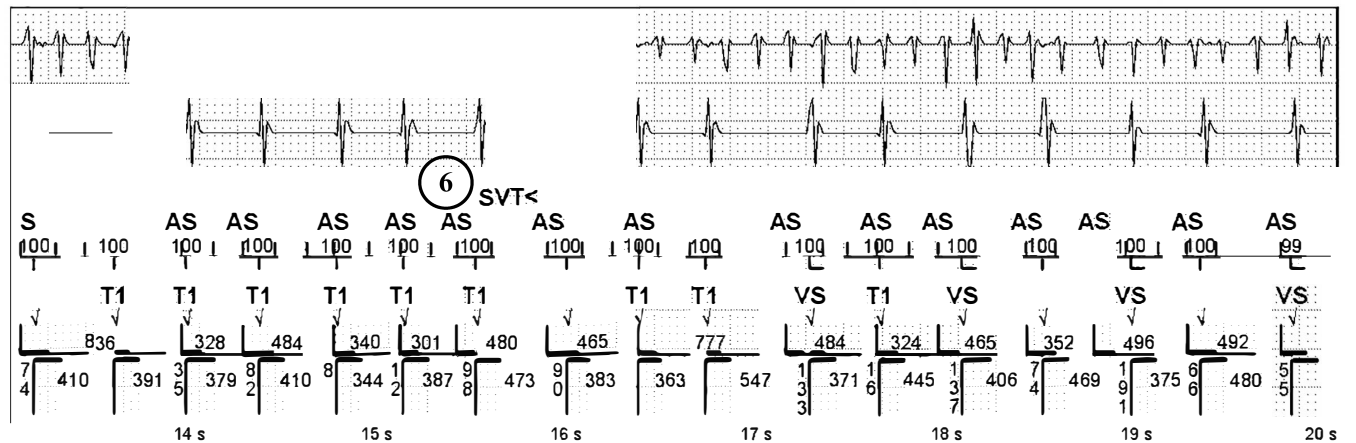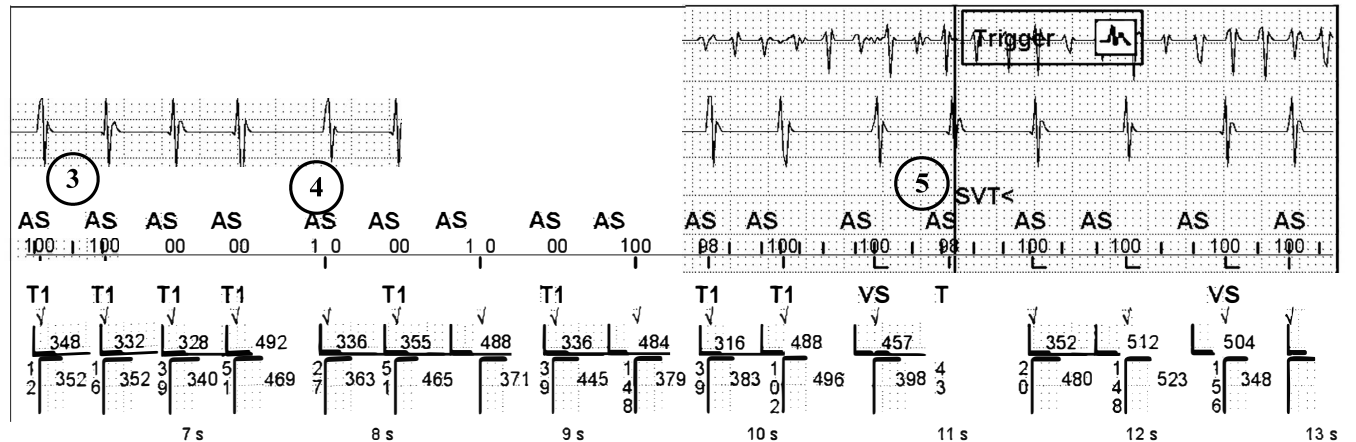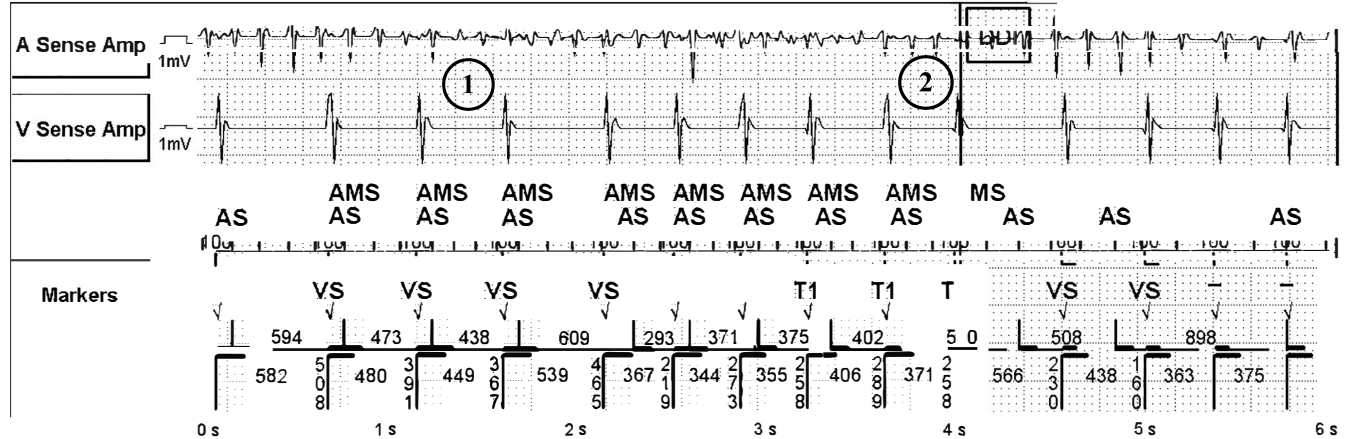



Episode: SVT (144 bpm / 415 ms) (Continued)

VT/VF Episode 42 of 63

Page 3 of 3

1: A Sense Amp AutoGain (1.4 mm/mV)

3: Markers

2: V Sense Amp AutoGain (0.4 mm/mV)

Sweep Speed: 25 mm/s

