



## Episode: VT-2 (190 bpm / 315 ms)

VT/VF Episode 1 of 3

Page 1 of 3

Duration 00:12 (M:S) No Alerts  
Detection Criteria 181 - 221 bpm

### Therapy

1) ATP

### Results

1) Below Rate Detection  
(CL 815 ms)

### ATP Therapy Details

#### VT-2 ATP Therapy

Successful BCL 272 ms

#### Therapy 1

Burst 1 272, 272, 272, 272, 272, 272, 272, 272, 272, 272,  
272 ms

### Diagnosis Summary

Diagnosis

#### VT-2

Time to Diagnosis 3.50 sec  
Rate (CL) 190 bpm (315 ms)  
Zone VT-2  
Rate Branch Classification VT (V > A) Rate Branch

### SVT Criteria Statistics

SVT Diagnoses during this episode 0

### DeFT Response™ Settings (Shock Waveform)

Waveform Biphasic  
Waveform Mode Tilt  
Shock Configuration RV to SVC & Can  
RV Polarity Anode(+)  
Defib Max Sensitivity 0.3 mV

VF Shocks (Defib)  
VT Shocks (CVRT)

#### 1st Phase

65 %  
Same as Defib

#### 2nd Phase

65 %  
Same as Defib

## Episode: VT-2 (190 bpm / 315 ms)

VT/VF Episode 1 of 3




Page 2 of 3

1: A Sense Amp AutoGain (1.1 mm/mV)

3: Markers

2: V Sense Amp AutoGain (0.4 mm/mV)

Sweep Speed: 25 mm/s

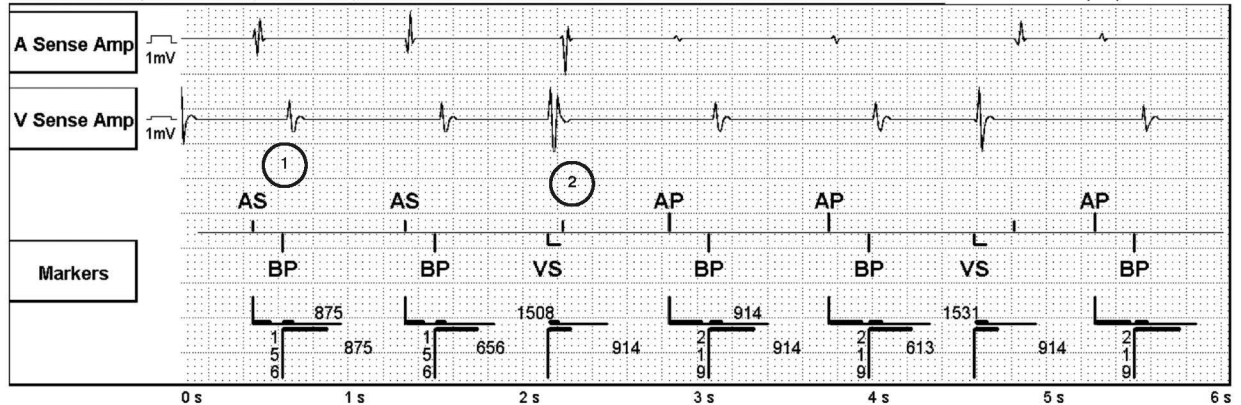

## Episode: VT-2 (190 bpm / 315 ms) (Continued)

VT/VF Episode 1 of 3


Page 3 of 3

1: A Sense Amp AutoGain (1.1 mm/mV)

3: Markers

2: V Sense Amp AutoGain (0.4 mm/mV)

Sweep Speed: 25 mm/s



## Episode: VT-2 (190 bpm / 315 ms)

VT/VF Episode 3 of 3

Page 1 of 3

Duration 00:12 (M:S) No Alerts  
Detection Criteria 181 - 221 bpm

### Therapy

1) ATP

### Results

1) Below Rate Detection  
(CL 815 ms)

### ATP Therapy Details

#### VT-2 ATP Therapy

Successful BCL 276 ms

#### Therapy 1

Burst 1 276, 276, 276, 276, 276, 276, 276, 276, 276, 276, 276 ms

### Diagnosis Summary

	Diagnosis
	VT-2
Time to Diagnosis	3.50 sec
Rate (CL)	190 bpm (315 ms)
Zone	VT-2
Rate Branch Classification	VT (V > A) Rate Branch

### SVT Criteria Statistics

SVT Diagnoses during this episode 0

### DeFT Response™ Settings (Shock Waveform)

			1st Phase	2nd Phase
Waveform	Biphasic	VF Shocks (Defib)	65 %	65 %
Waveform Mode	Tilt	VT Shocks (CVRT)	Same as Defib	Same as Defib
Shock Configuration	RV to SVC & Can			
RV Polarity	Anode(+)			
Defib Max Sensitivity	0.3 mV			



## Episode: VT-2 (190 bpm / 315 ms)

VT/VF Episode 3 of 3




Page 2 of 3

1: A Sense Amp AutoGain (1.0 mm/mV)

3: Markers

2: V Sense Amp AutoGain (0.4 mm/mV)

Sweep Speed: 25 mm/s



# Episode: VT-2 (190 bpm / 315 ms) (Continued)

VT/VF Episode 3 of 3


Page 3 of 3

1: A Sense Amp AutoGain (1.0 mm/mV)

3: Markers

2: V Sense Amp AutoGain (0.4 mm/mV)

Sweep Speed: 25 mm/s



## Episode: VT-2 (190 bpm / 315 ms)

VT/VF Episode 2 of 3

Page 1 of 3

Duration 00:12 (M:S) No Alerts  
Detection Criteria 181 - 221 bpm

### Therapy

1) ATP

### Results

1) Below Rate Detection  
(CL 795 ms)

### ATP Therapy Details

#### VT-2 ATP Therapy

Successful BCL 276 ms

#### Therapy 1

Burst 1 276, 276, 276, 276, 276, 276, 276, 276, 276, 276,  
276 ms

### Diagnosis Summary

	Diagnosis
	VT-2
Time to Diagnosis	3.50 sec
Rate (CL)	190 bpm (315 ms)
Zone	VT-2
Rate Branch Classification	VT (V > A) Rate Branch

### SVT Criteria Statistics

SVT Diagnoses during this episode 0

### DeFT Response™ Settings (Shock Waveform)

			1st Phase	2nd Phase
Waveform	Biphasic	VF Shocks (Defib)	65 %	65 %
Waveform Mode	Tilt	VT Shocks (CVRT)	Same as Defib	Same as Defib
Shock Configuration	RV to SVC & Can			
RV Polarity	Anode(+)			
Defib Max Sensitivity	0.3 mV			



## Page 2 of 3

Sweep Speed: 25 mm/s

## Episode: VT-2 (190 bpm / 315 ms) (Continued)

VT/VF Episode 2 of 3

Page 3 of 3

1: A Sense Amp AutoGain (0.9 mm/mV)

3: Markers

2: V Sense Amp AutoGain (0.4 mm/mV)

Sweep Speed: 25 mm/s

