

Episode: VT-2 (222 bpm / 270 ms)

VT/VF Episode 1 of 6

Page 1 of 3

Duration 00:16 (M:S)
Detection Criteria 176 - 229 bpm

Alerts



Three or more VT/VF episodes in 24 hours

Therapy

1) ATP

Results

1) Below Rate Detection
(CL 505 ms)

ATP Therapy Details

VT-2 ATP Therapy

Successful BCL 228 ms

Therapy 1

Burst 1 228, 228, 228, 228, 228, 228, 228, 228 ms

Diagnosis Summary

	Diagnosis
	VT-2
Time to Diagnosis	9.25 sec
Rate (CL)	222 bpm (270 ms)
Zone	VT-2
VT Diagnosis Criteria	Any
Rate Branch Classification	Sinus Tach (V = A) Rate Branch

Morphology

On, ≥ 60% is a match, ≥ 5 matches indicate SVT
Min Match Score n/a
Max Non-Match Score 0%
No. Template Matches 0 of 8 **(VT Indicated)**

Sudden Onset

On, < 100 ms indicates SVT
Max Delta 275 ms **(VT Indicated)**

SVT Criteria Statistics

SVT Diagnoses during this episode 0

Measured SVT Discriminator values through initial VT/VF Diagnosis

Min Match Score	n/a	Max Non-Match Score	0 %
Template Used	19 Apr 2011 14:46	Max Onset Delta	275 ms

DeFT Response™ Settings (Shock Waveform)

Waveform	Biphasic	VF Shocks (Defib)	1st Phase	2nd Phase
Waveform Mode	Tilt	VT Shocks (CVRT)	65 %	65 %
Shock Configuration	RV to Can		Same as Defib	Same as Defib
RV Polarity	Anode(+)			
Defib Max Sensitivity	0.5 mV			

Episode: VT-2 (222 bpm / 270 ms)

VT/VF Episode 1 of 6




Page 2 of 3

1: A Sense Amp AutoGain (1.2 mm/mV)

3: Markers

2: V Sense Amp AutoGain (0.4 mm/mV)

Sweep Speed: 25 mm/s

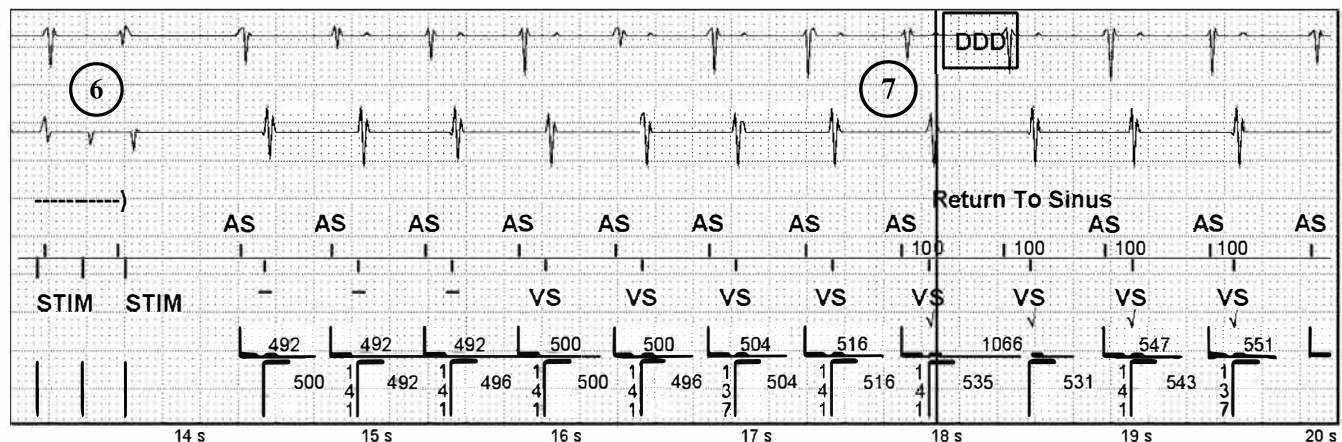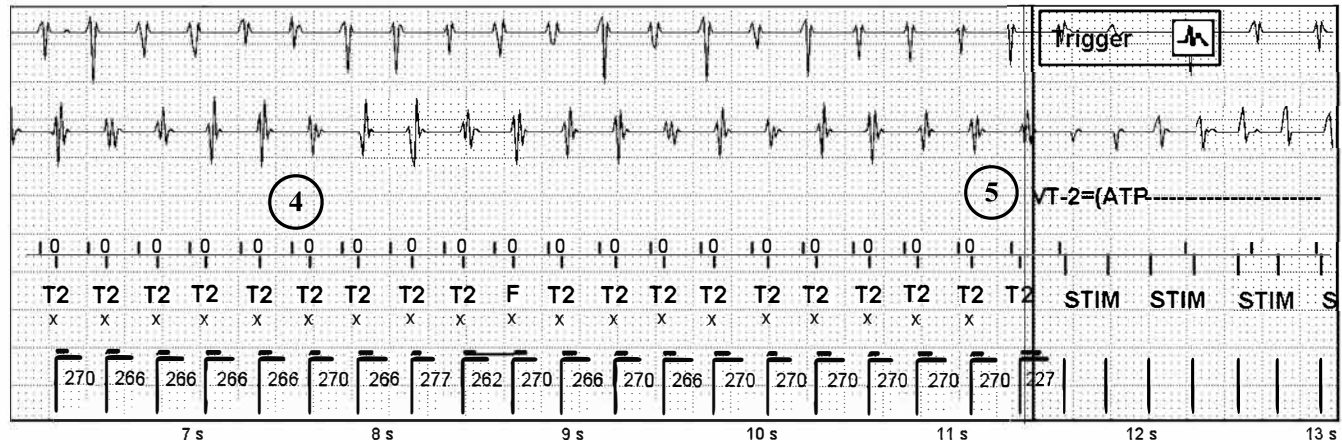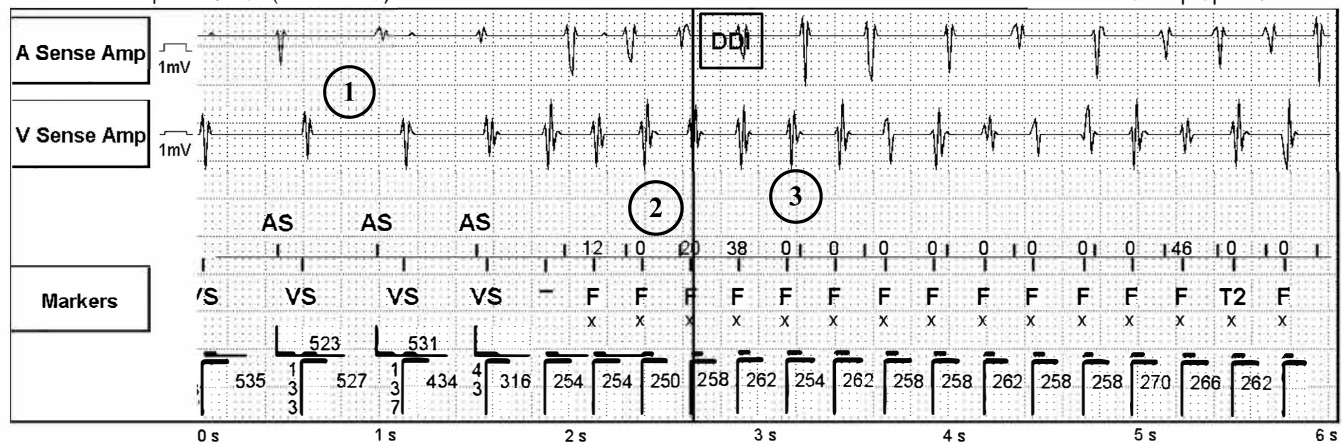



Episode: VT-2 (222 bpm / 270 ms) (Continued)

VT/VF Episode 1 of 6

Page 3 of 3

1: A Sense Amp AutoGain (1.2 mm/mV)

3: Markers

2: V Sense Amp AutoGain (0.4 mm/mV)

Sweep Speed: 25 mm/s

