





FVT Episode n° 1

N°	Type	Date	Time hh:mm	Duration hh:mm:ss	Max V Rate	Median V Rate
----	------	------	---------------	----------------------	------------	---------------


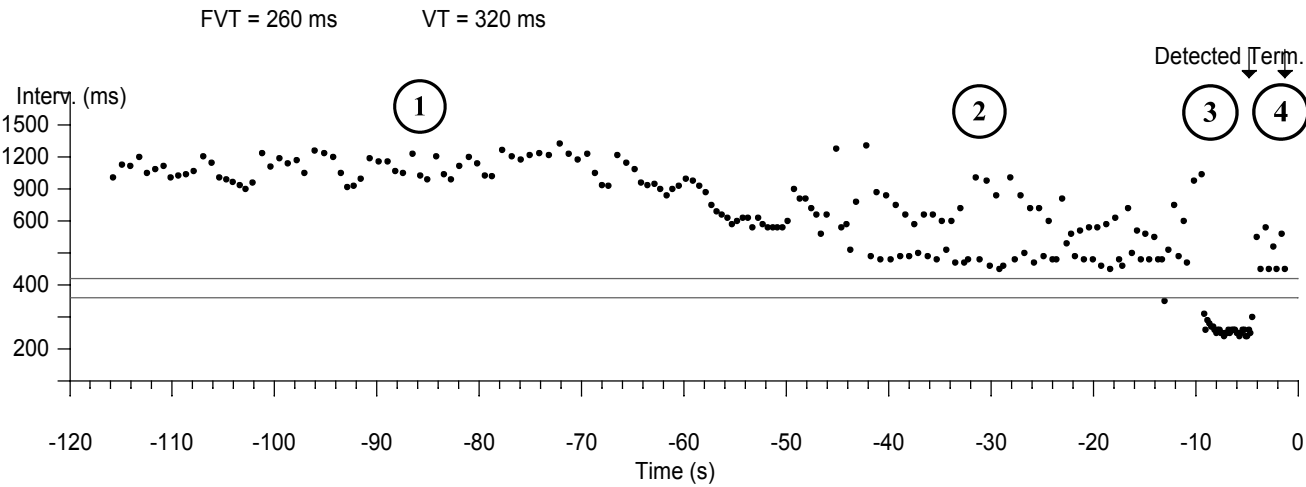


FVT Episode n° 1

Serial number :

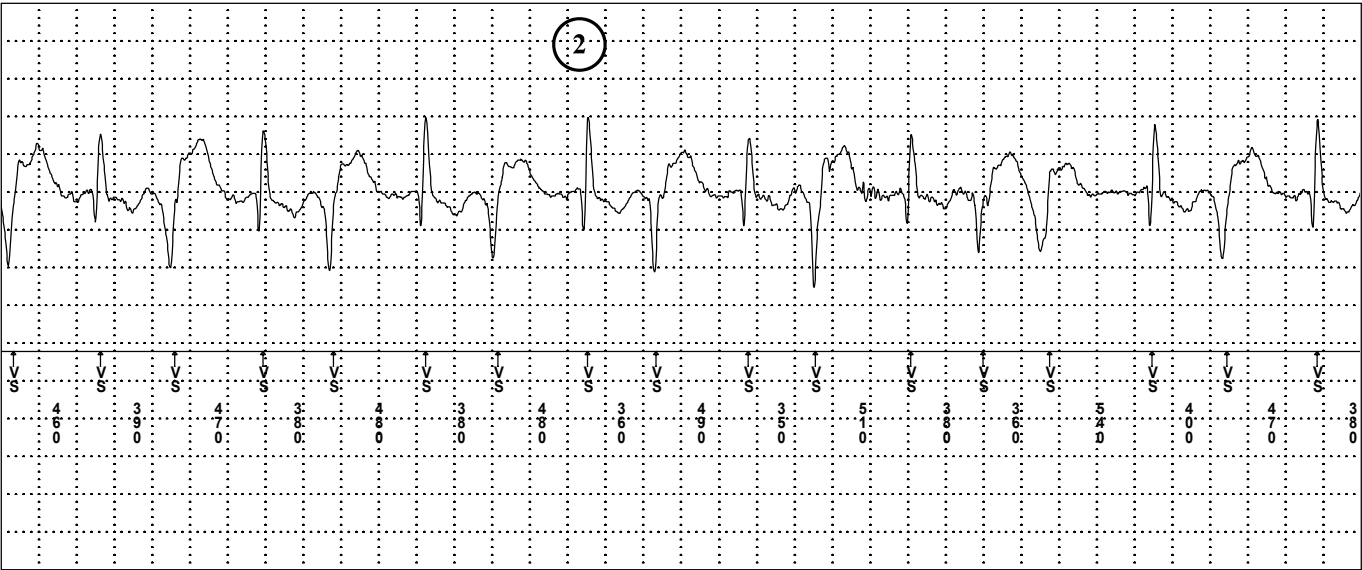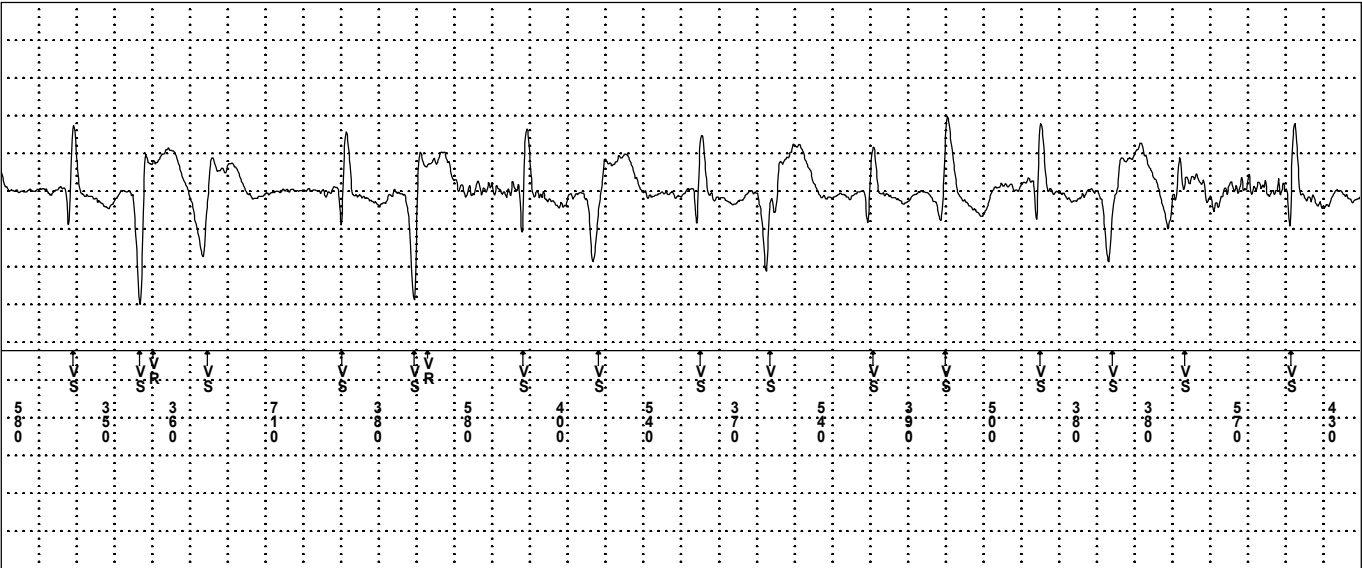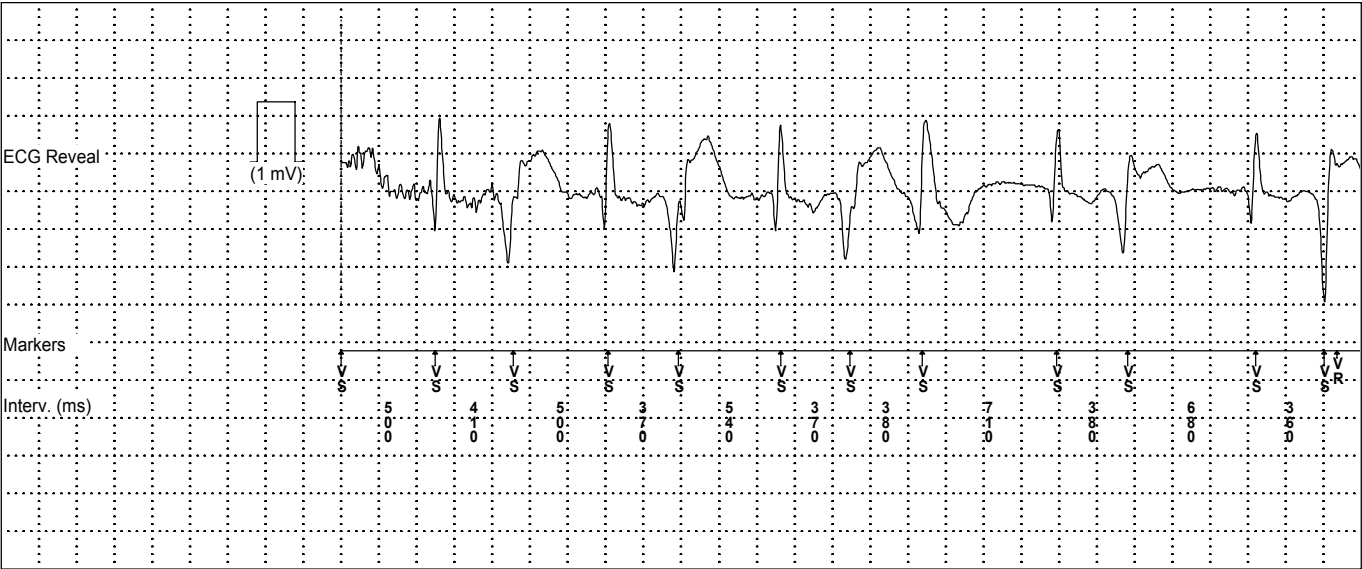

FVT Episode n° 1

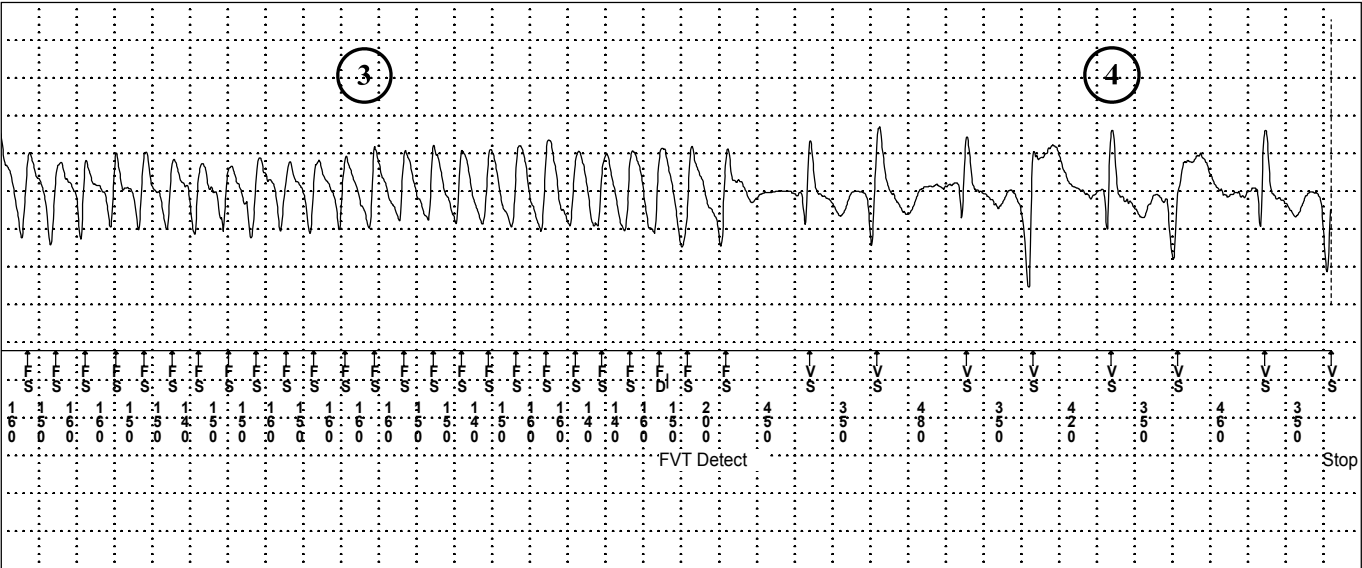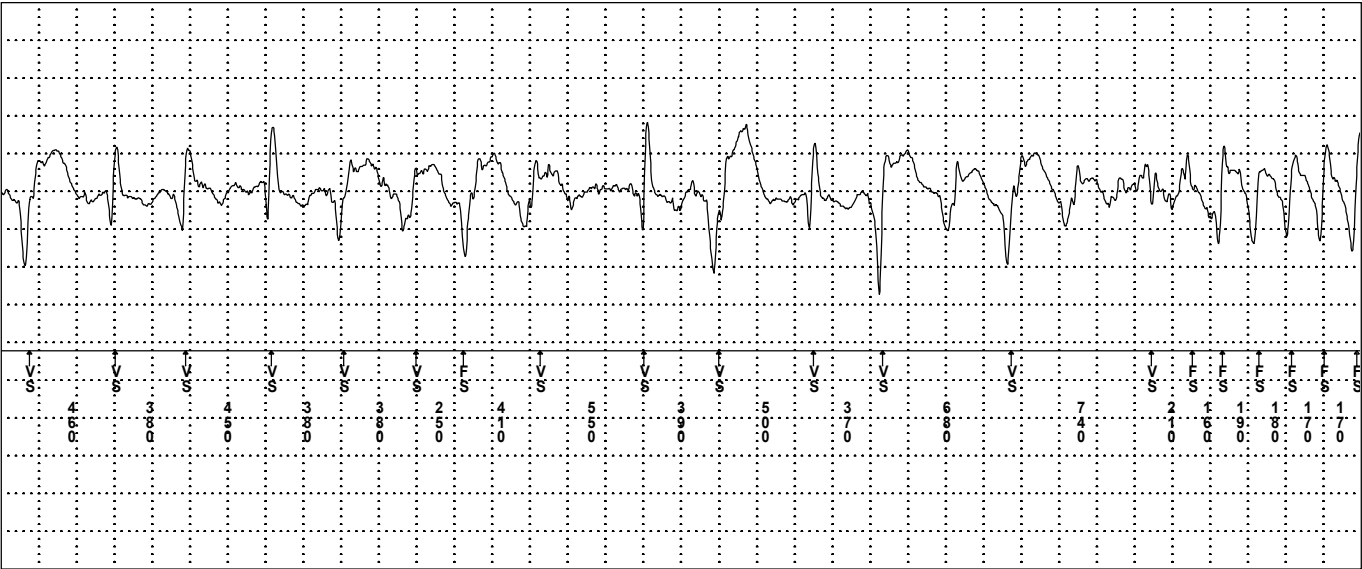

FVT Episode n° 1

Episode #1 :

Episode Summary

Type	FVT
Duration	5 s
Max V.Rate	400 bpm (150 ms)
Médian V. Rate	375 bpm (160 ms)
Average V. Rate	400 bpm (150 ms)
Activity Level	Active

Parameter Settings	ECG recording	Interval V. (rate)	Duration
FVT	On	260 ms (231 bpm)	30/40 beats.
VT	On	320 ms (188 bpm)	16 beats.

Detection Enhancements

VT Detection		
	Stability VT	Off
	Onset VT	Off

Sensing

Sensibility	0.035 mV (35 μ V)
Sensing Threshold Decay Delay	100 ms