




Device: **Reveal® XT 9529**

Date of Interrogation:

ID#	Type	Date	Time hh:mm	Duration hh:mm:ss	Max V. Rate	Median V. Rate
720	Brady	08-Jul-	20:00	:24	Min <30 bpm	<30 bpm (>2000 ms)

Brady = 2000 ms



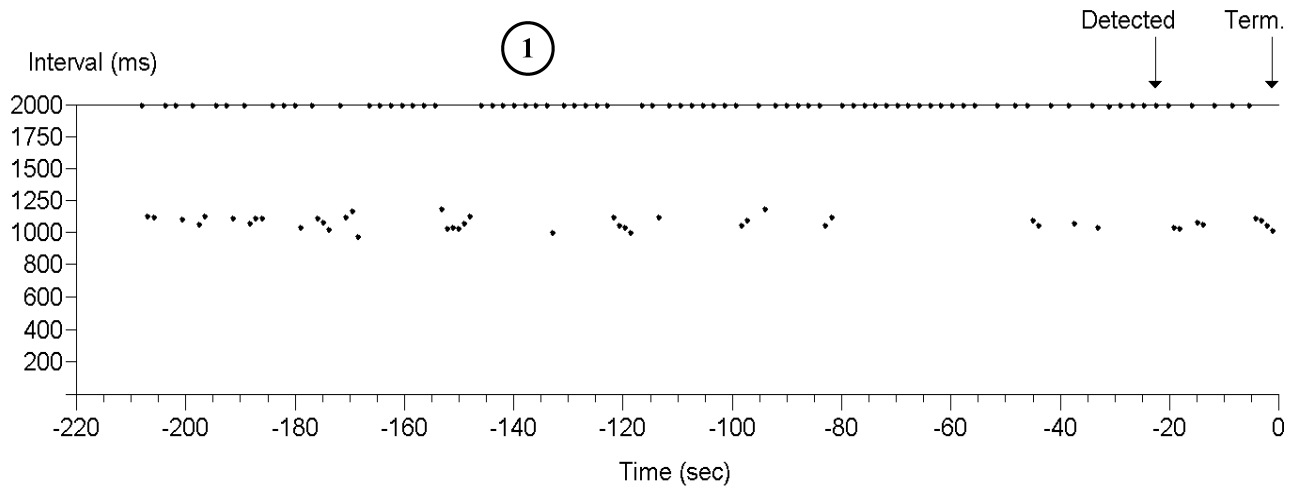




Device: Reveal® XT 9529

Date of Interrogation:

Episode #720 Chart speed: 25.0 mm/sec

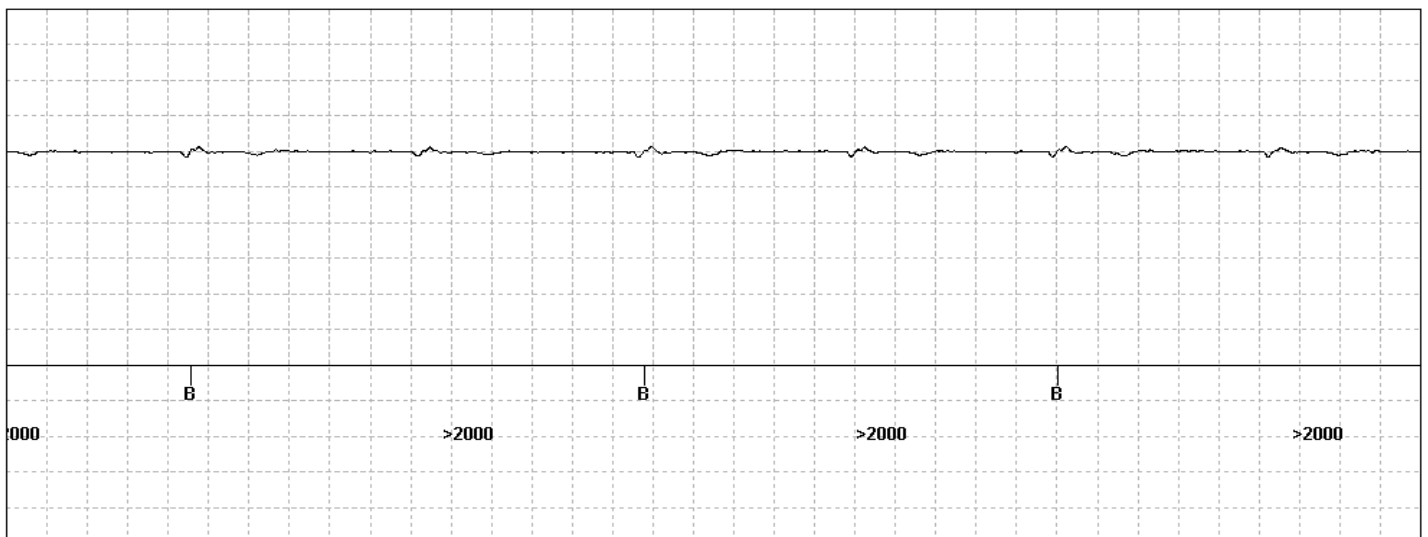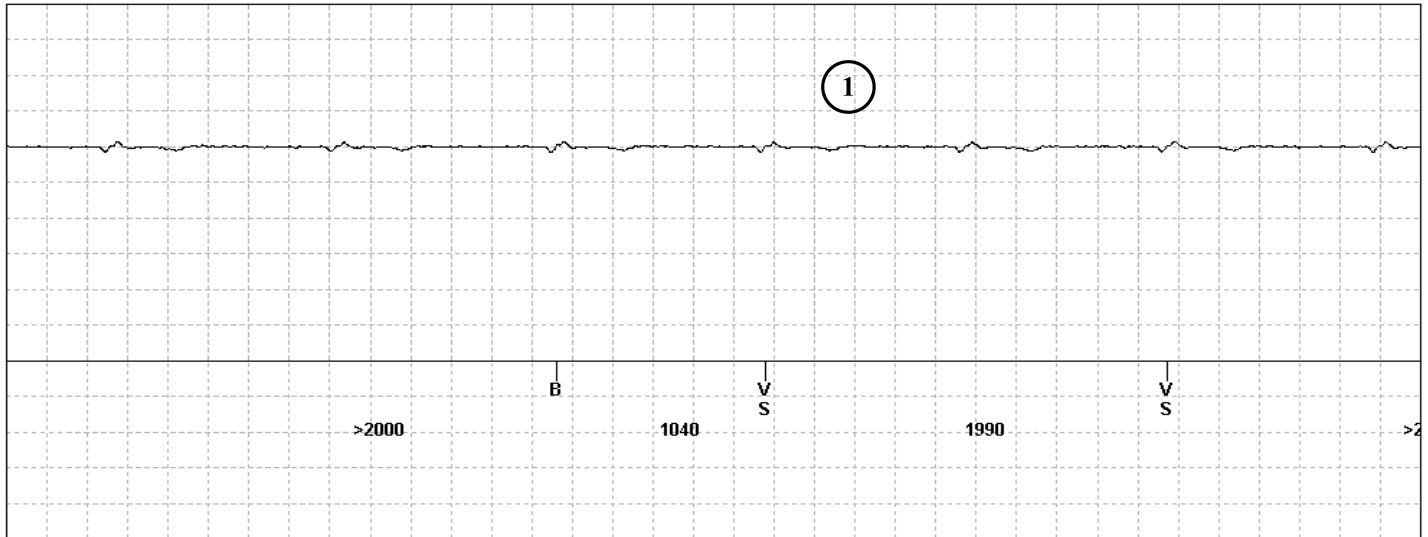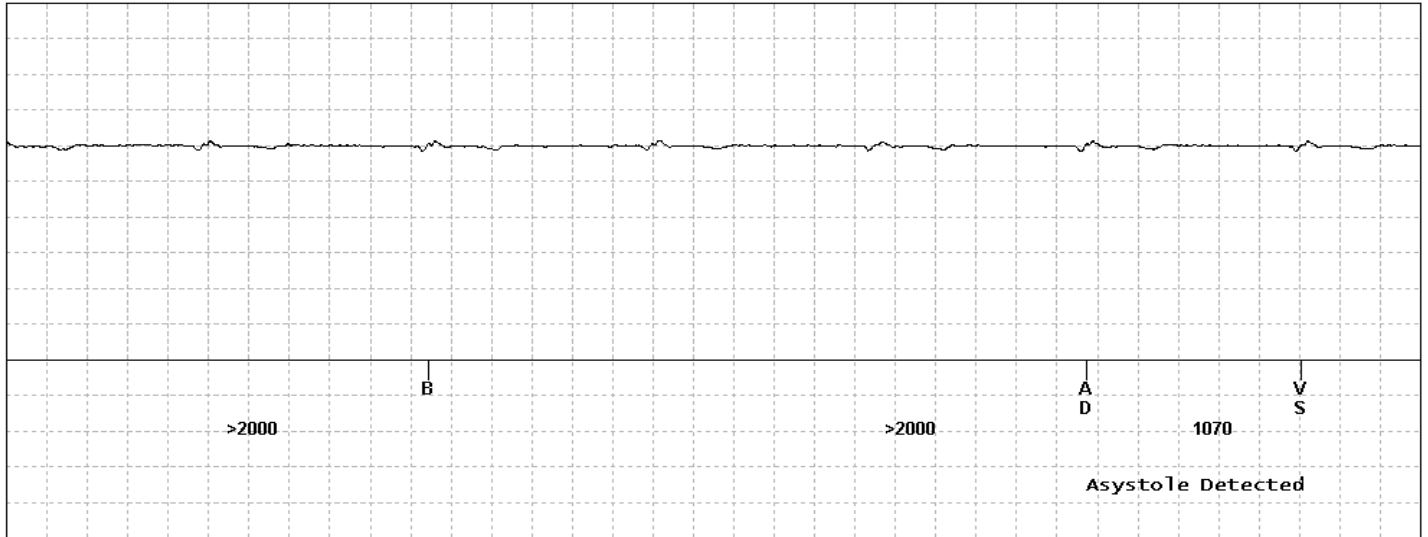

Device: **Reveal® XT 9529**

Date of Interrogation:

Physician:

Episode #720:**Episode Summary**

Type	Brady
Duration	24 sec
Min V. Rate	<30 bpm (>2000 ms)
Median V. Rate	<30 bpm (>2000 ms)
Average V. Rate	<30 bpm (>2000 ms)
Activity Level	Inactive

Parameter Settings	ECG Recording	V. Interval (Rate)	Duration
Brady	On	2000 ms (30 bpm)	4 beats

Sensing

Sensitivity	0.025 mV (25 µV)
Sensing Threshold Decay Delay	100 ms