




Device: **Reveal® XT 9529**

Date of Interrogation:

ID#	Type	Date	Time hh:mm	Duration hh:mm:ss	Max V. Rate	Median V. Rate
694	AF	05-Jul-2	07:10	:22:00	125 bpm (480 ms)	61 bpm (990 ms)



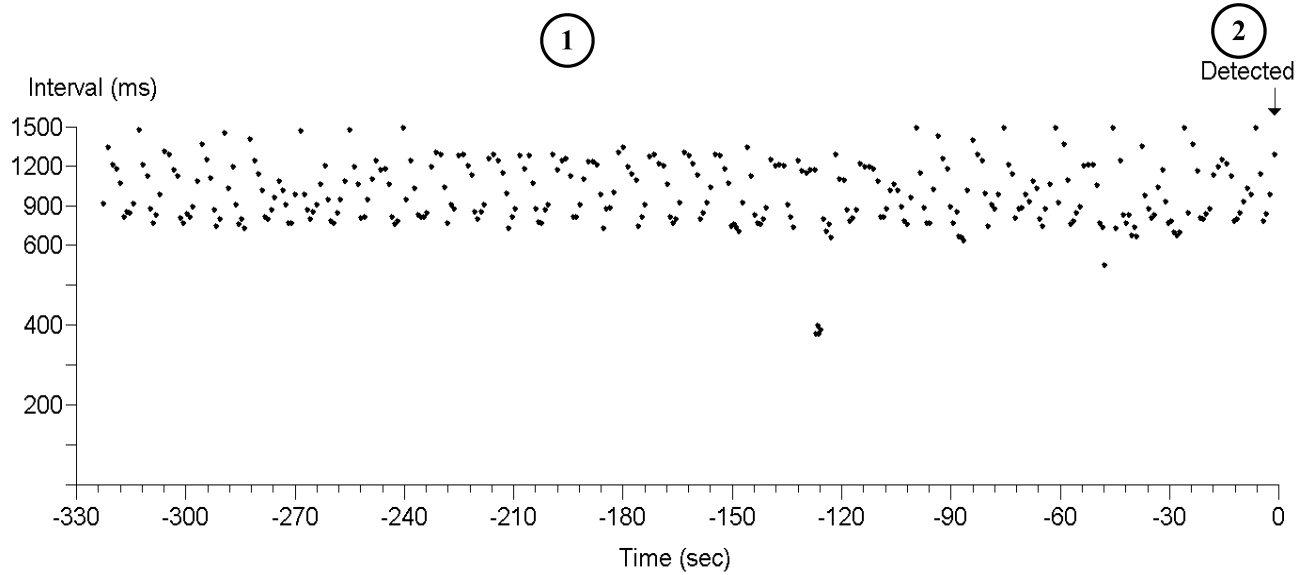




Device: Reveal® XT 9529

Date of Interrogation:

Episode #694 Chart speed: 25.0 mm/sec

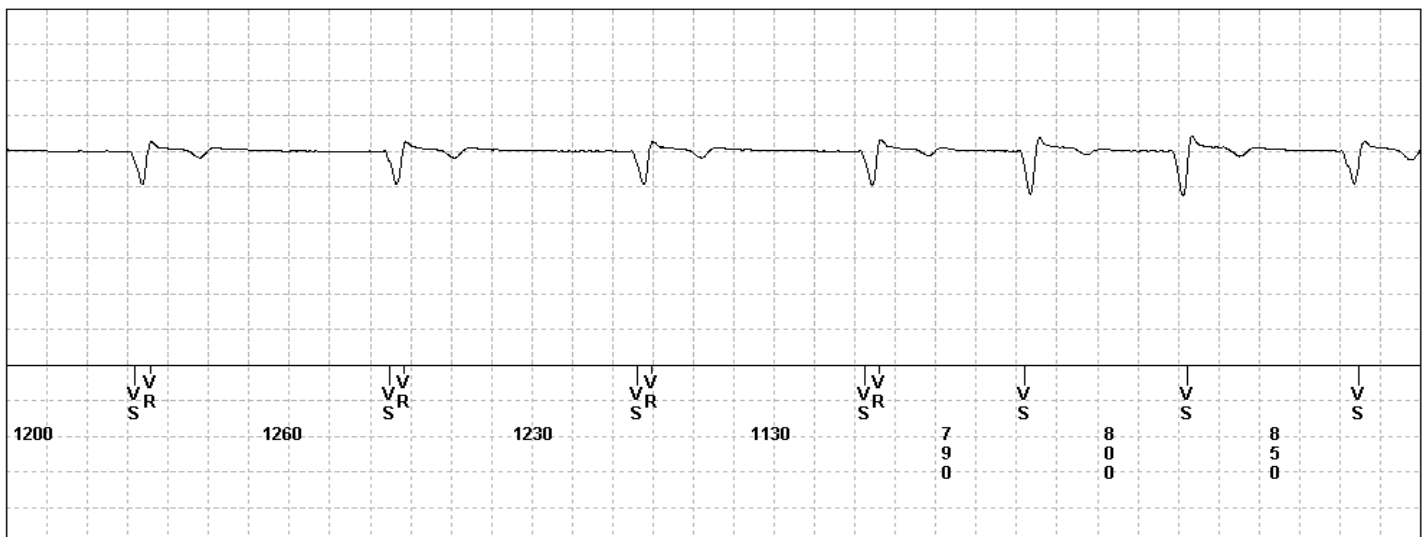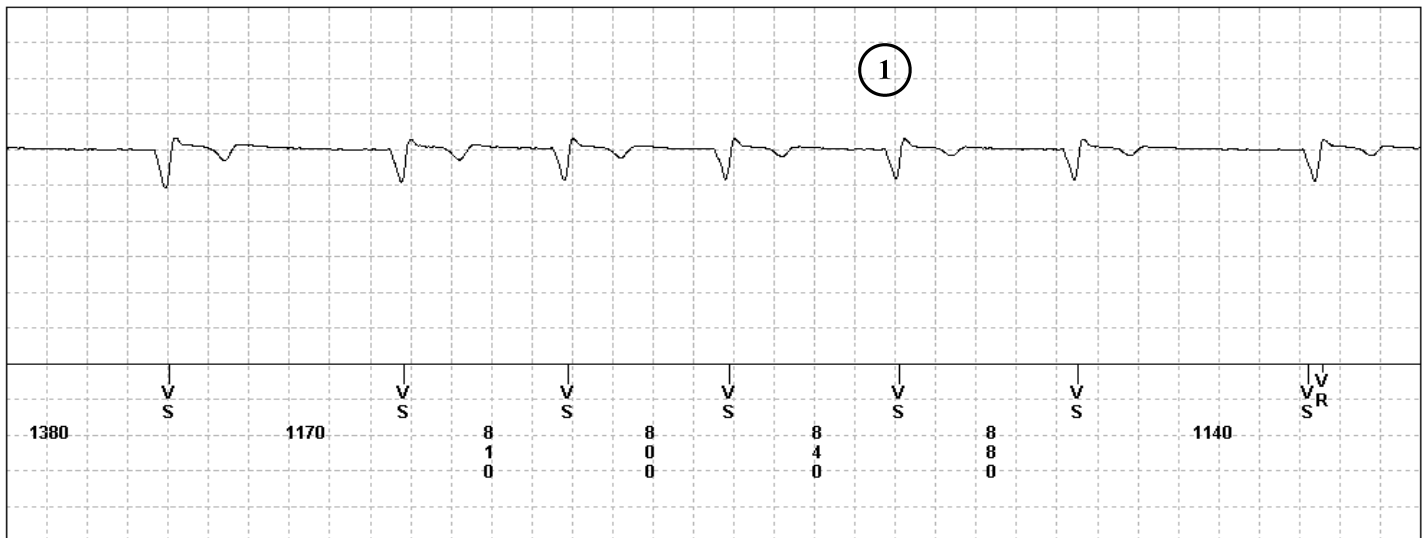
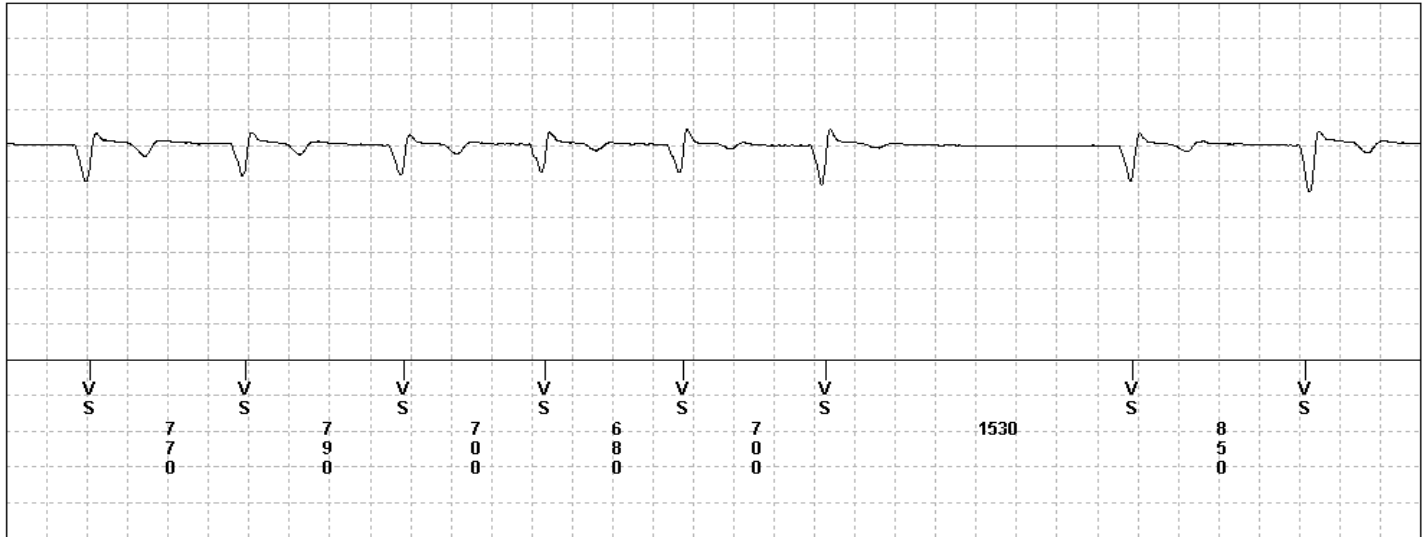




Device: Reveal® XT 9529

Date of Interrogation:

Episode #694 Chart speed: 25.0 mm/sec

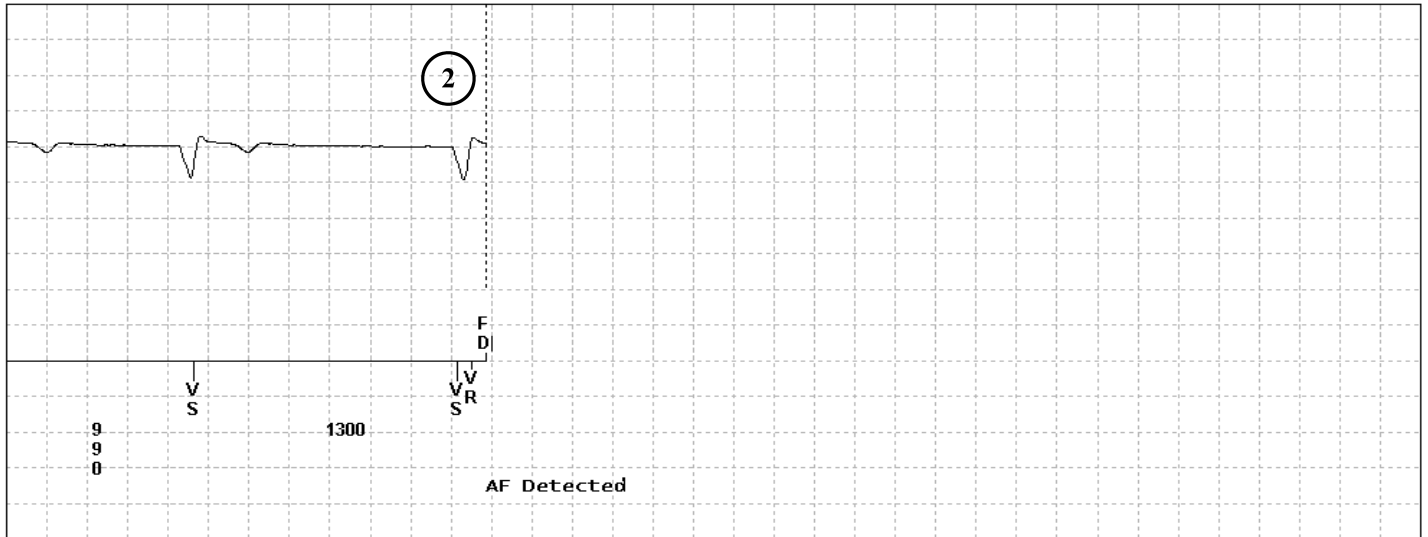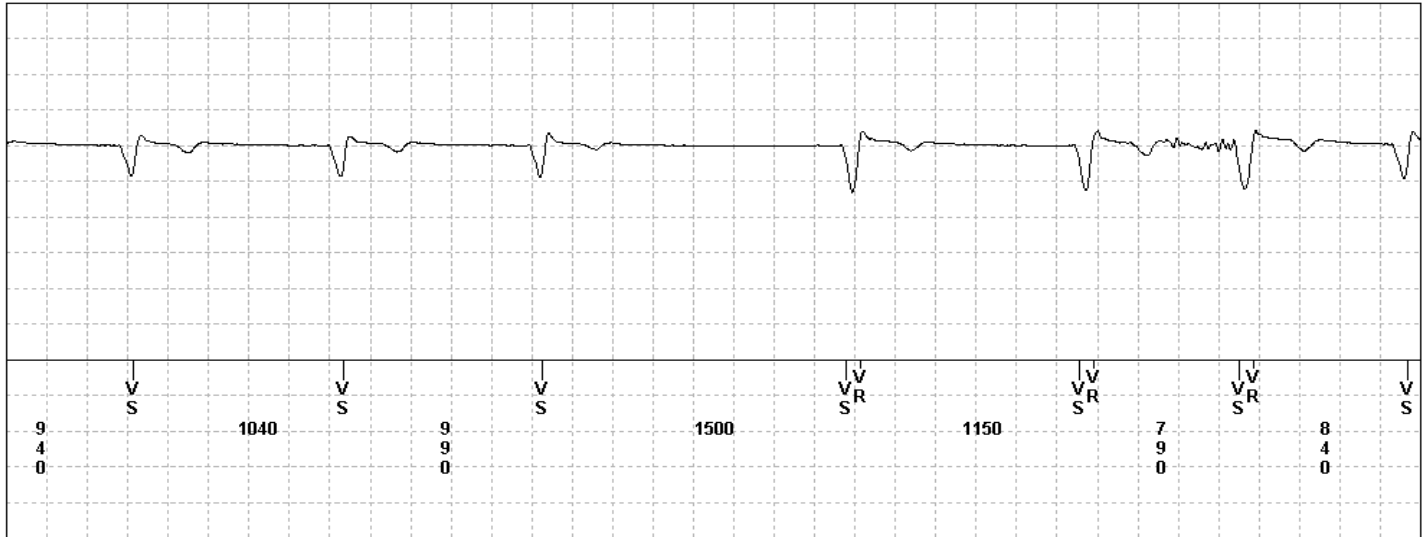

Device: **Reveal® XT 9529**

Date of Interrogation:

Physician:

**Episode #694:****Episode Summary**

Type	AF
Duration	22 min
Max V. Rate	125 bpm (480 ms)
Median V. Rate	61 bpm (990 ms)
Activity Level	Inactive

**Parameter Settings    ECG Recording**

AT/AF	On
-------	----

**Detection Enhancements**

AT/AF Detection	Type	AF Only
	AF Detection	Balanced Sensitivity
	Ectopy Rejection	Off

**Sensing**

Sensitivity	0.025 mV (25 µV)
Sensing Threshold Decay Delay	100 ms