

Treated VT/VF Episode #43

Device: **EnTrust D154VRC**

Serial Number:

Date of Visit: **20-Jun-2005 12:21:53**


Patient:

ID:

Physician:

Type	ATP Seq	Shocks	Success	ID#	Date	Time hh:mm	Duration hh:mm:ss	Avg bpm V	Max bpm V	Activity at Onset
VT	1		Yes	43	19-Jun-2005	21:32	:06	188	188	Active

• V-V VF = 320 ms FVT = 280 ms VT = 400 ms

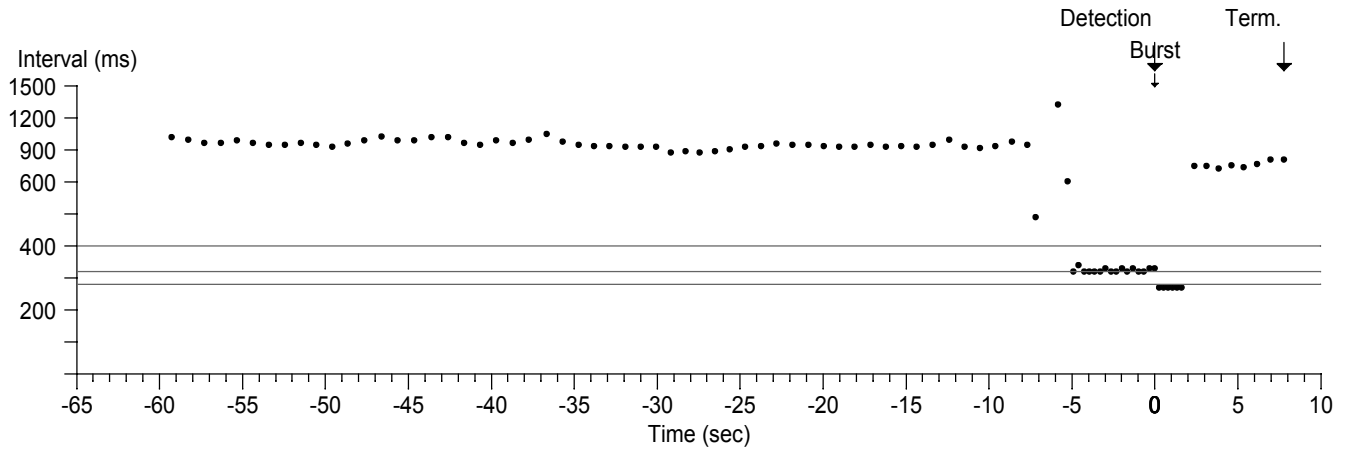

Patient:

ID:

Episode #43 - VT Chart speed: 25.0 mm/sec

