

Treated VT/VF Episode #18

Device: **Virtuoso DR D164AWG**

Serial Number:

Date of Visit: **17-Jun-2014 15:28:46**

Patient:

ID:

Physician:

Type	ATP Seq	Shocks	Success	ID#	Date	Time hh:mm	Duration hh:mm:ss	Avg bpm A/V	Max bpm A/V	Activity at Onset
VF	1	35J	Yes	18	08-Jan-2014	11:57	:26	115/240	---/---	Active

• V-V

□ A-A

VF = 320 ms


FVT = 260 ms

VT = 370 ms

Detection

Burst

Term.

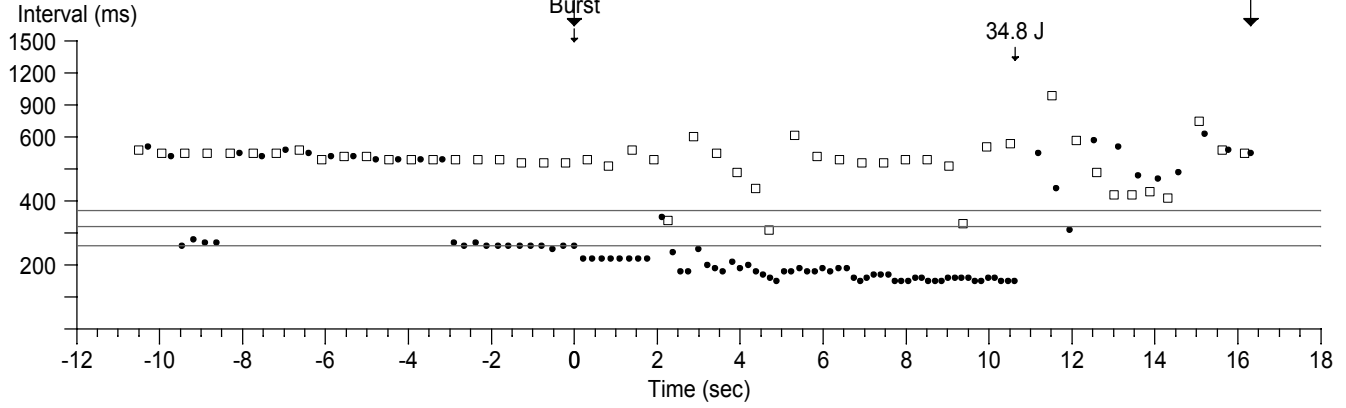

Treated VT/VF Episode #18

Device: **Virtuoso DR D164AWG**



Serial Number:

Date of Visit: **17-Jun-2014 15:28:46**

Patient:

ID:

Episode #18 - VF Chart speed: 25.0 mm/sec

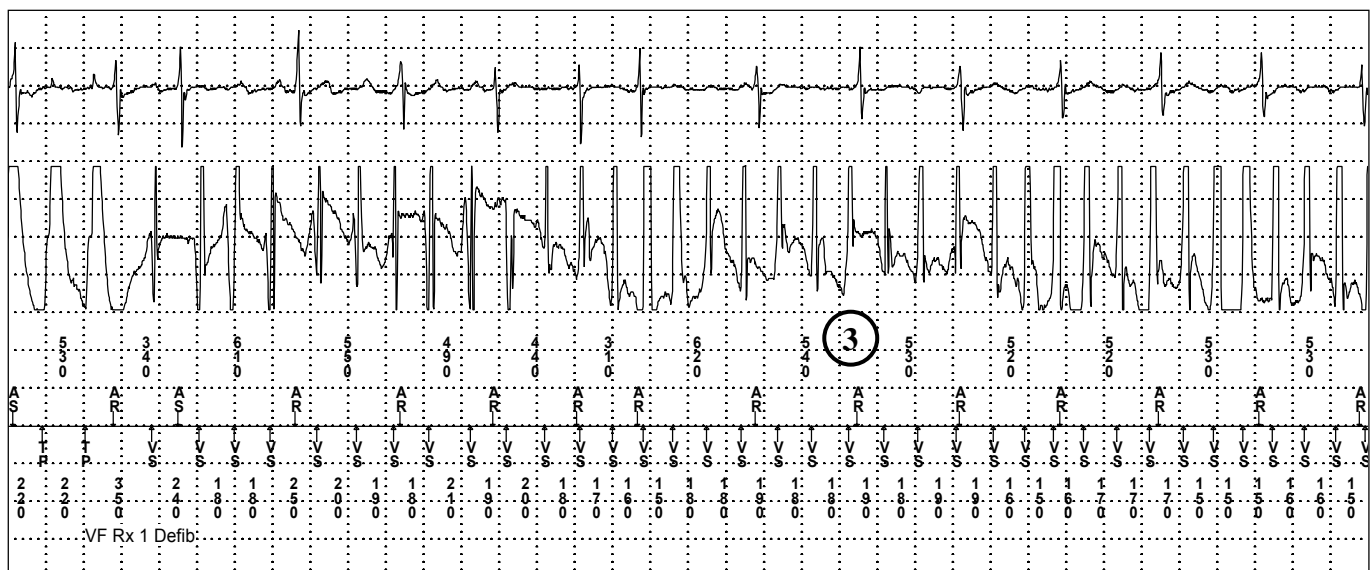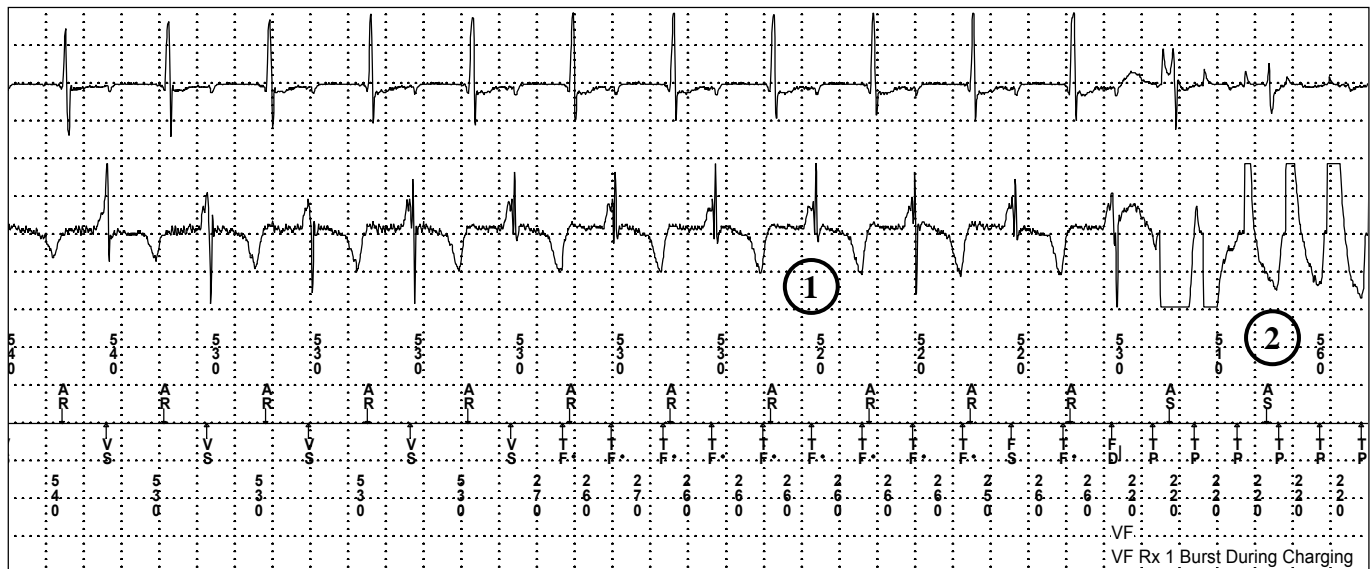

Treated VT/VF Episode #18

Device: **Virtuoso DR D164AWG**

Serial Number:

Date of Visit: **17-Jun-2014 15:28:46**

Patient:

ID:

Episode #18 - VF Chart speed: 25.0 mm/sec

