

Non-sustained High Rate Episode #2

Device: **Evera XT DR DDBB2D1**

Serial Number:

Date of Visit: **12-Sep-2016 14:37:56**

Patient:

ID:

Physician:


Type	ATP Seq	Shocks	Success	ID#	Date	Time hh:mm	Duration hh:mm:ss	Avg bpm A/V	Max bpm A/V	Activity at Onset
High Rate-NS				2	10-Sep-2016	16:46	:01	269/305		Rest

• V-V

□ A-A

VF = 300 ms

Term.

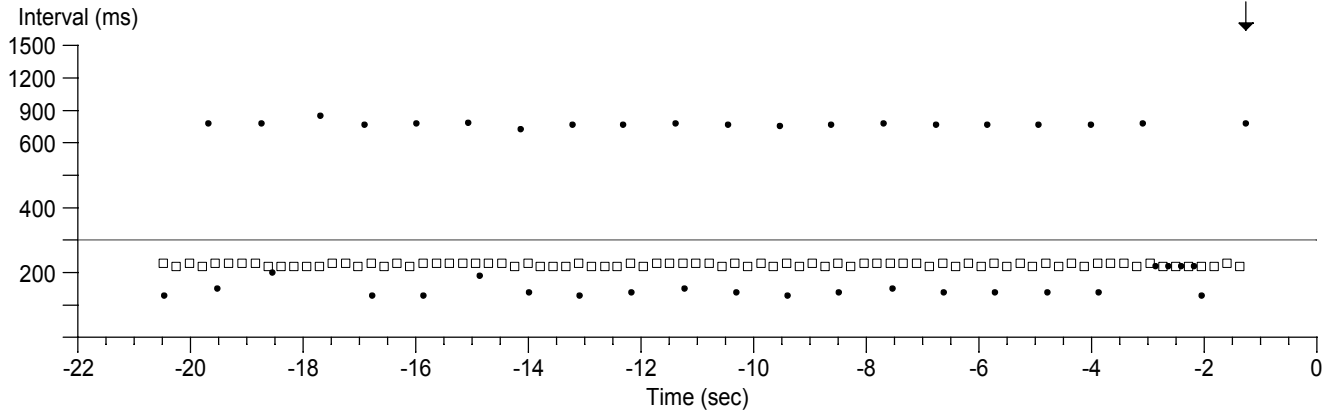

Episode #2 Chart speed: 25.0 mm/sec

Non-sustained High Rate Episode #2

Device: **Evera XT DR DDBB2D1**

Serial Number:

Date of Visit: **12-Sep-2016 14:37:56**

Patient:

ID:

Episode #2 Chart speed: 25.0 mm/sec

