

# Treated VT/VF Episode #1

Device: **Evera XT DR DDBB2D1**

Serial Number:

Date of Visit: **11-Dec-2015 11:29:42**

Patient:

ID:


Physician:

Type	ATP Seq	Shocks	Success	ID#	Date	Time hh:mm	Duration hh:mm:ss	Avg bpm A/V	Max bpm A/V	Activity at Onset
VF	0	35J,35J	No	1	08-Dec-2015	16:30	:40	---/240	---/286	Active

• V-V

□ A-A

VF = 300 ms

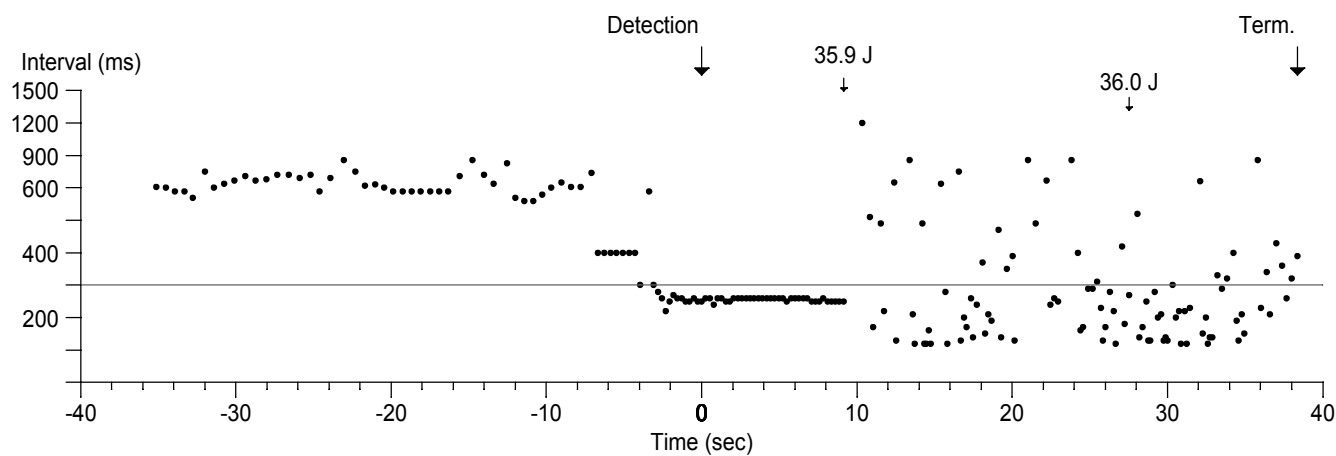

# Treated VT/VF Episode #1

Device: **Evera XT DR DDBB2D1**




Serial Number:

Date of Visit: **11-Dec-2015 11:29:42**

Patient:

ID:

**Episode #1 - VF** Chart speed: 25.0 mm/sec

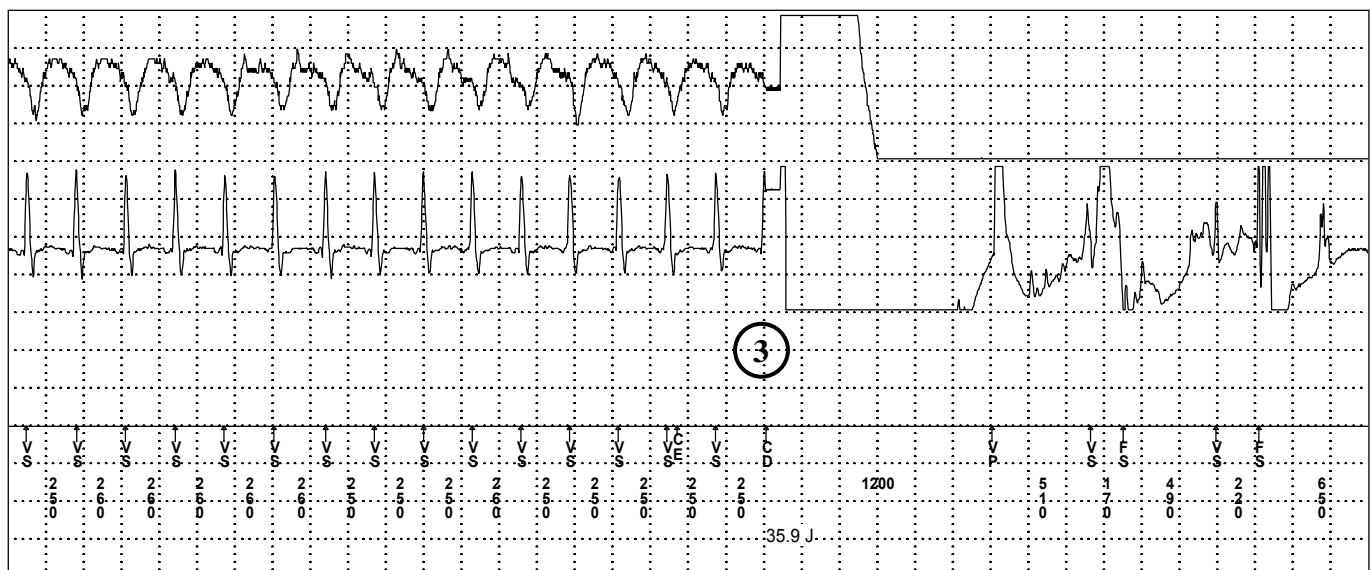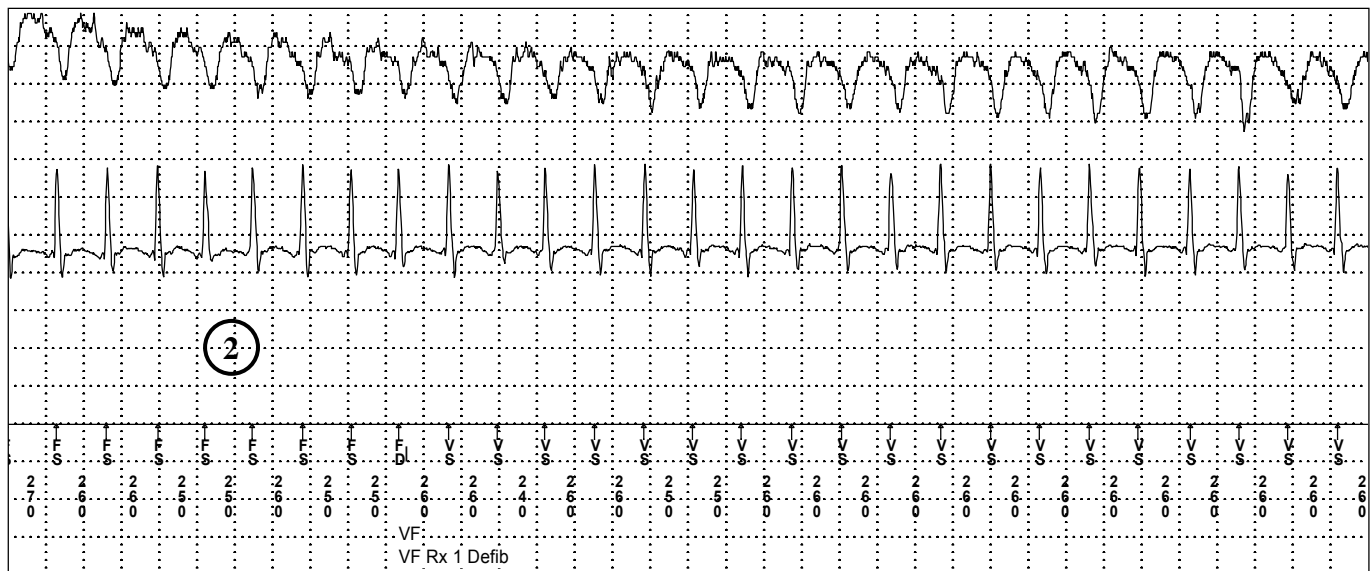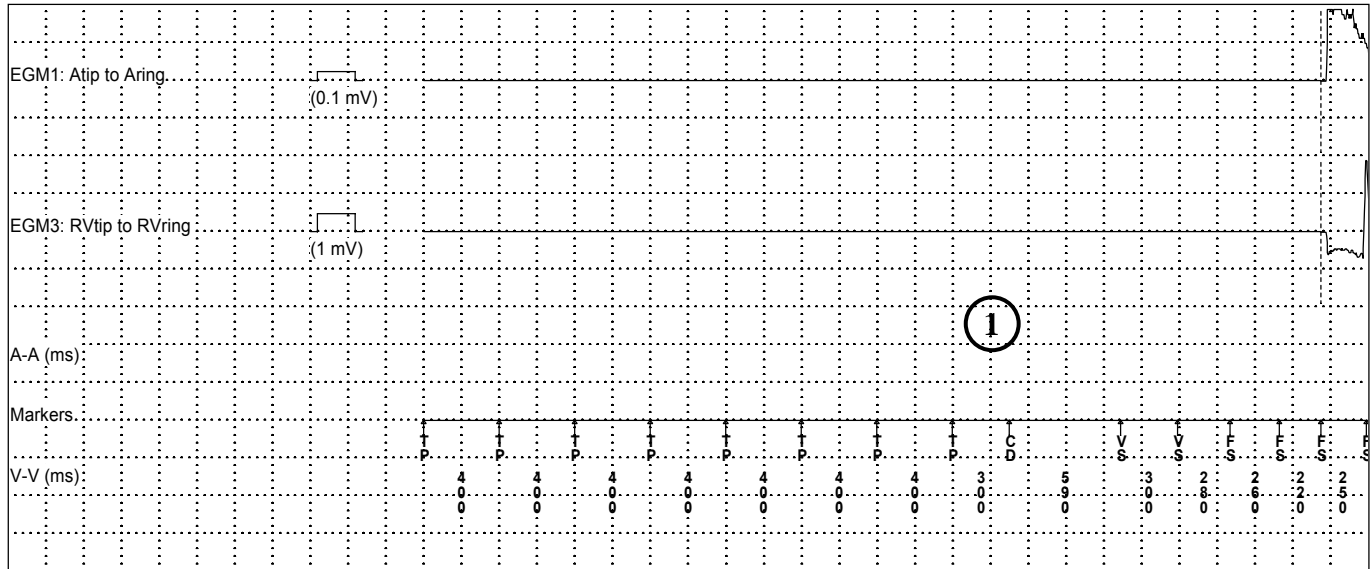

# Treated VT/VF Episode #1

Device: **Evera XT DR DDBB2D1**




Serial Number:

Date of Visit: **11-Dec-2015 11:29:42**

Patient:

ID:

Episode #1 - VF Chart speed: 25.0 mm/sec

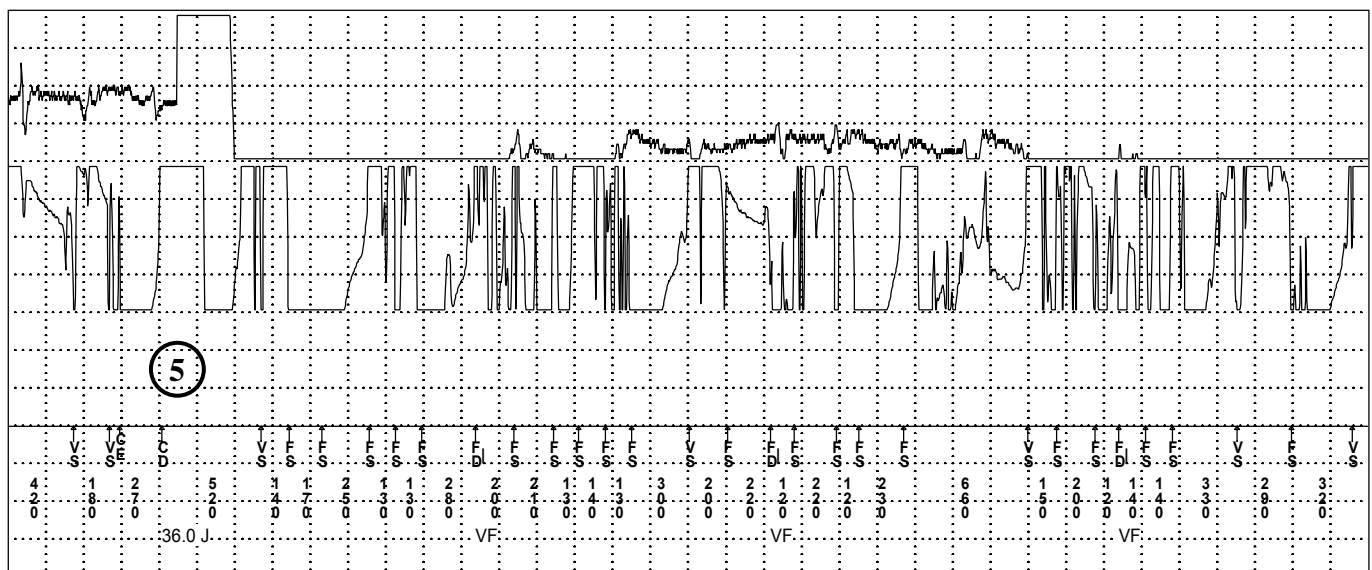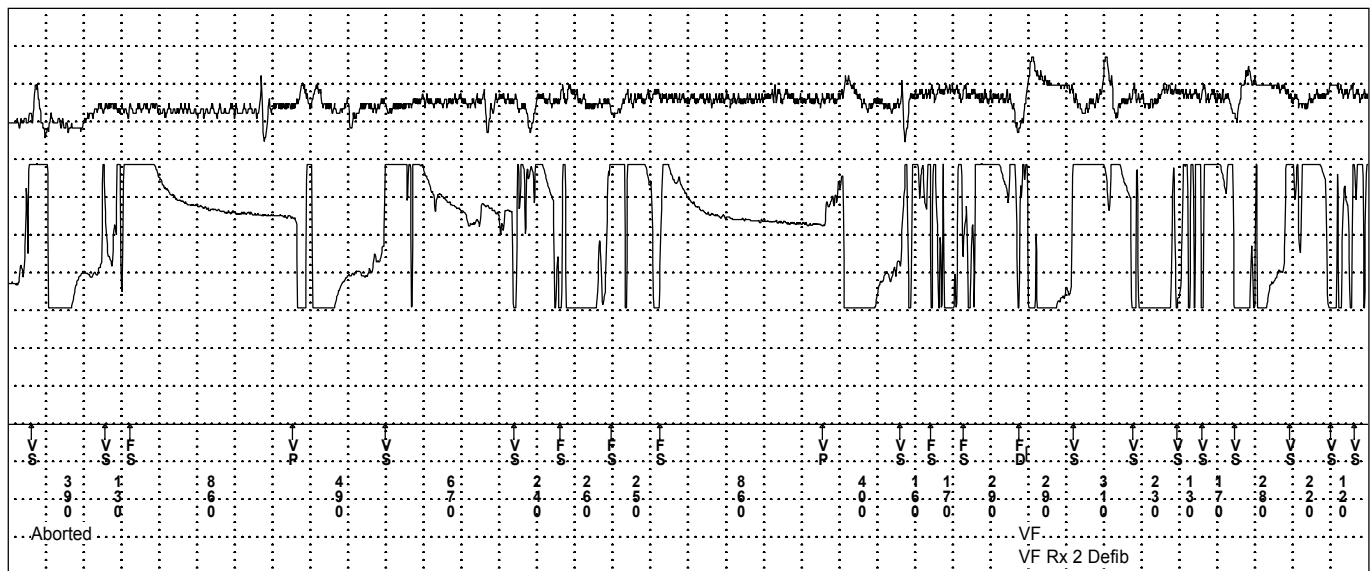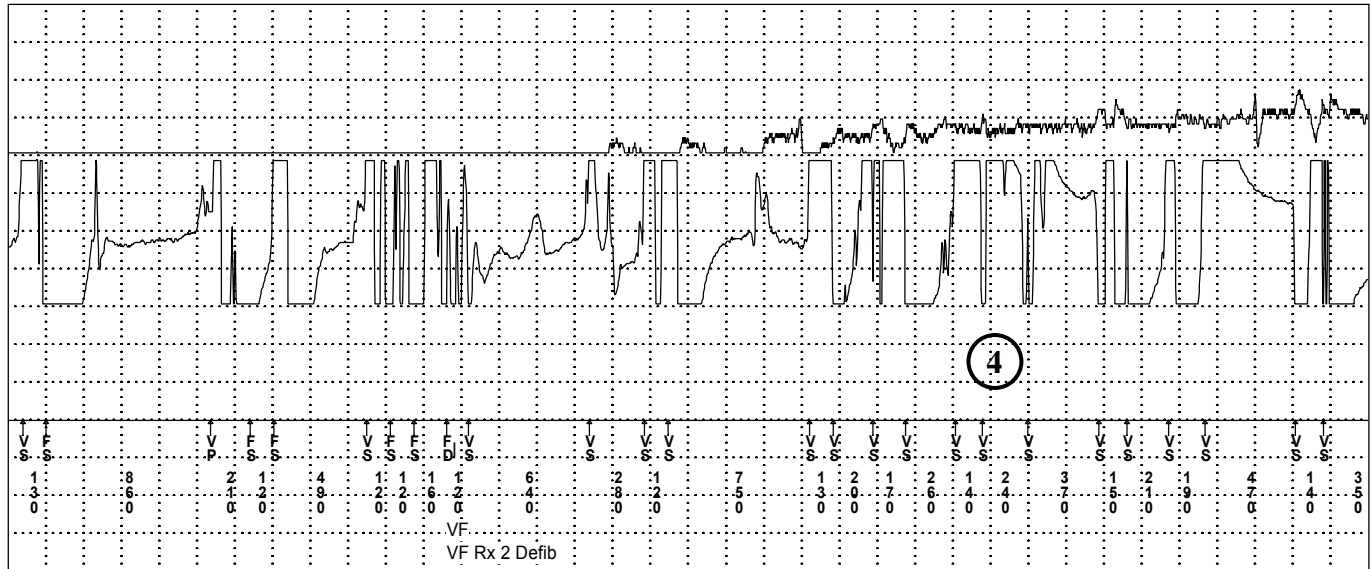

# Treated VT/VF Episode #1

Device: **Evera XT DR DDBB2D1**

Serial Number:

Date of Visit: **11-Dec-2015 11:29:42**

Patient:

ID:

**Episode #1 - VF Chart speed: 25.0 mm/sec**

