

SVT Episode #24

Device: **EnTrust D154ATG**

Serial Number:

Date of Visit: **26-Nov-2007 16:15:19**

Patient:

ID:

Physician:

Type	ATP Seq	Shocks	Success	ID#	Date	Time hh:mm	Duration hh:mm:ss	Avg bpm A/V	Max bpm A/V	Activity at Onset
SVT-Onset				24	25-Nov-2007	07:52	:09:45	82/143	97/146	Rest


• V-V

□ A-A

VF = 320 ms

VT = 430 ms

VT/VF Detection Withheld

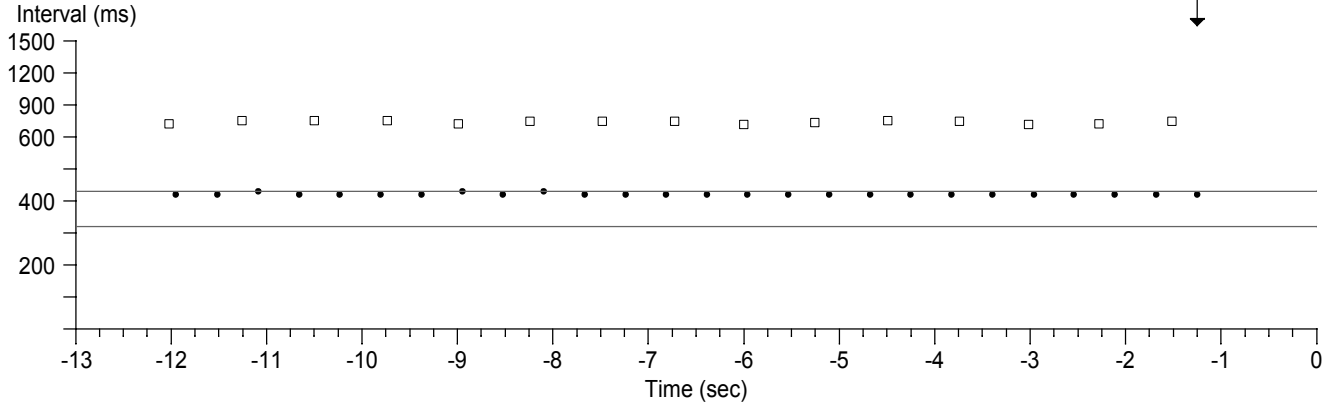

SVT Episode #24

Device: **EnTrust D154ATG**


Serial Number:

Date of Visit: **26-Nov-2007 16:15:19**

Patient:

ID:

Episode #24 Chart speed: 25.0 mm/sec

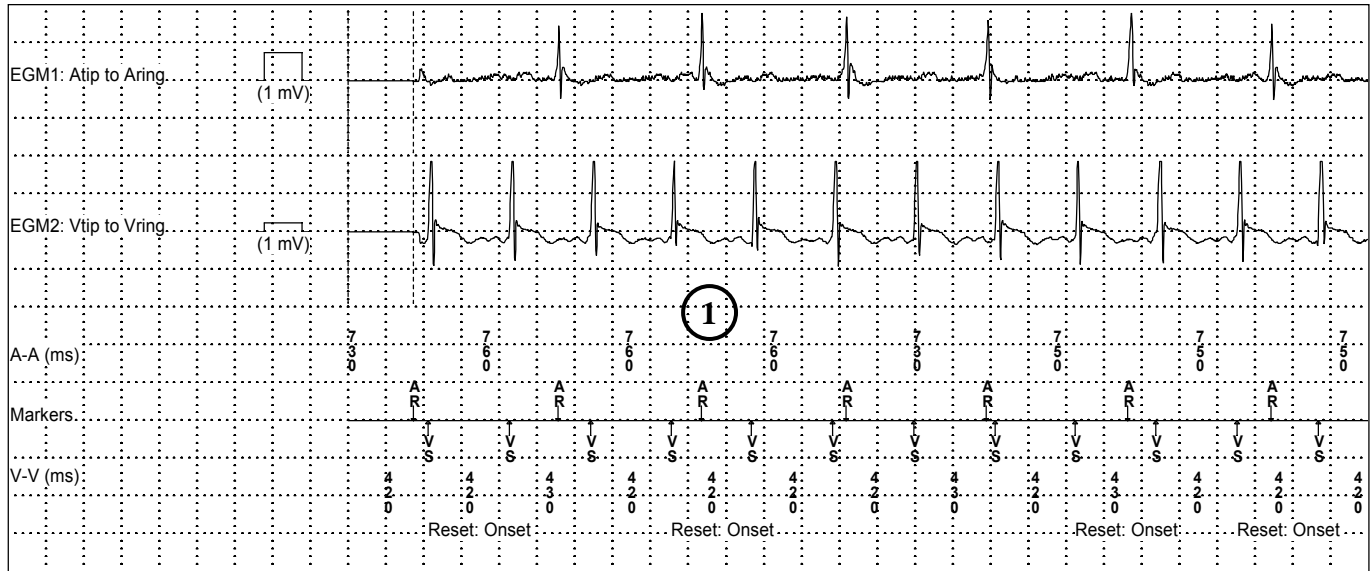

SVT Episode #24

Device: **EnTrust D154ATG**

Serial Number:

Date of Visit: **26-Nov-2007 16:15:19**

Patient:

ID:

Physician:

Episode #24: 25-Nov-2007 07:52:23

Episode Summary

Initial Type SVT - Onset (spontaneous)
Duration 9.8 min
A/V Max Rate 97 bpm/146 bpm
V. Median 143 bpm (420 ms)
Activity at onset Rest, Sensor = 79 bpm
Episode transitioned to a VT/VF episode.

SVT Criteria Triggered

Onset

Parameter Settings Initial Redetect V. Interval (Rate)

VF	On	12/16	9/12	320 ms (188 bpm)
FVT	Off			
VT	On	16	12	430 ms (140 bpm)
Monitor	Off	20		

PR Logic

AF/Afl	On
Sinus Tach	On
Other 1:1 SVTs	Off
SVT V. Limit	320 ms

Other Enhancements

Stability	40 ms
Onset	On (81%)
High Rate Timeout	Off

2

EGM EGM1 EGM2 Sensitivity

Source	Atip to Aring	Vtip to Vring	Atrial	0.3 mV
Range	+/- 8 mV	+/- 8 mV	RV	0.3 mV