



Device: Virtuoso™ II VR D294VRC

Serial Number:

Date of Interrogation: 03-Nov-2014 23:26:09


Patient:

Physician:

Type	ATP Seq	Shocks	Success	ID#	Date	Time hh:mm	Duration hh:mm:ss	Avg bpm V	Max bpm V	Activity at Onset
VF	0	35J, 35J	Yes	9	13-Jun-2014	17:14	:23	375	---	Active

• V-V

VF = 290 ms FVT = 250 ms VT = 330 ms

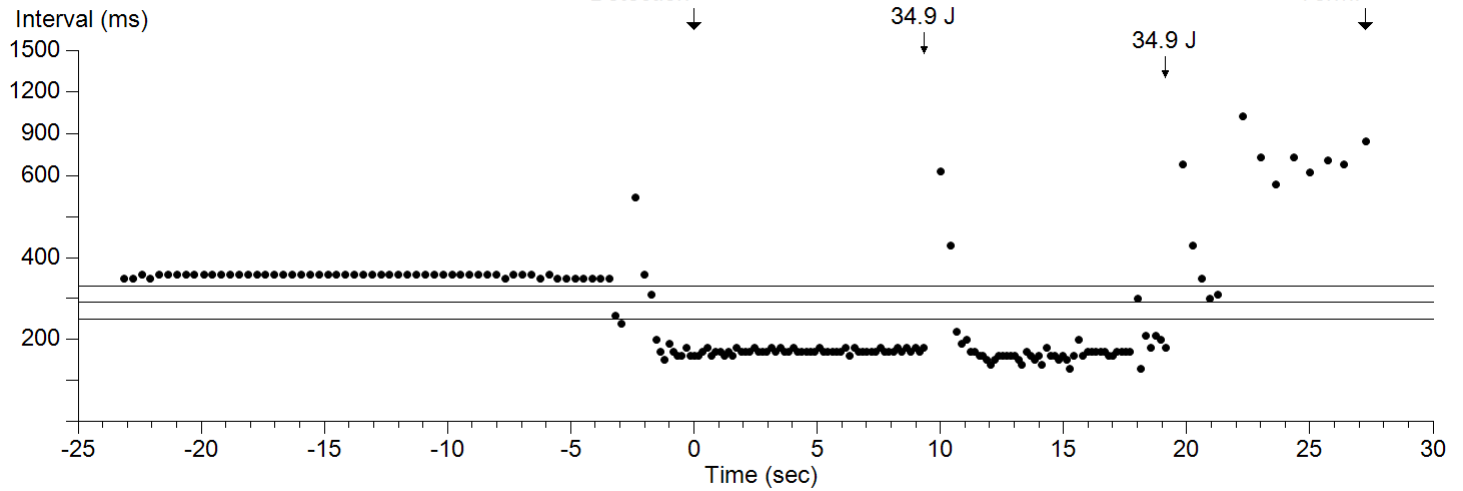



Treated VT/VF Episode #9

Episode #9 - VF Chart speed: 25.0 mm/sec





Treated VT/VF Episode #9

Episode #9 - VF Chart speed: 25.0 mm/sec

