



**ZOOM® View™ DISK**  
**Selected Episodes Report**

Device TELIGEN  
Tachy Mode Monitor + Therapy

**Event V-54: 08 Aug 2012 09:35**

**VF Event Onset**

Avg V Rate: 237 bpm

Detection: Rhythm ID

**At V-Detect**

Avg V Rate: 259 bpm

Rate Zone: VF

RhythmID Correlated: False

SRD Met: (False, Off)

ATP Timeout: False

**Attempt 1, 41 J V Shock**

Elapsed Time: 00:00:03


**Shock Information:**


Charge Time: 8.5 s

Lead Impedance: 59  $\Omega$

Lead Polarity: Initial


**Event Ended 00:00:43**

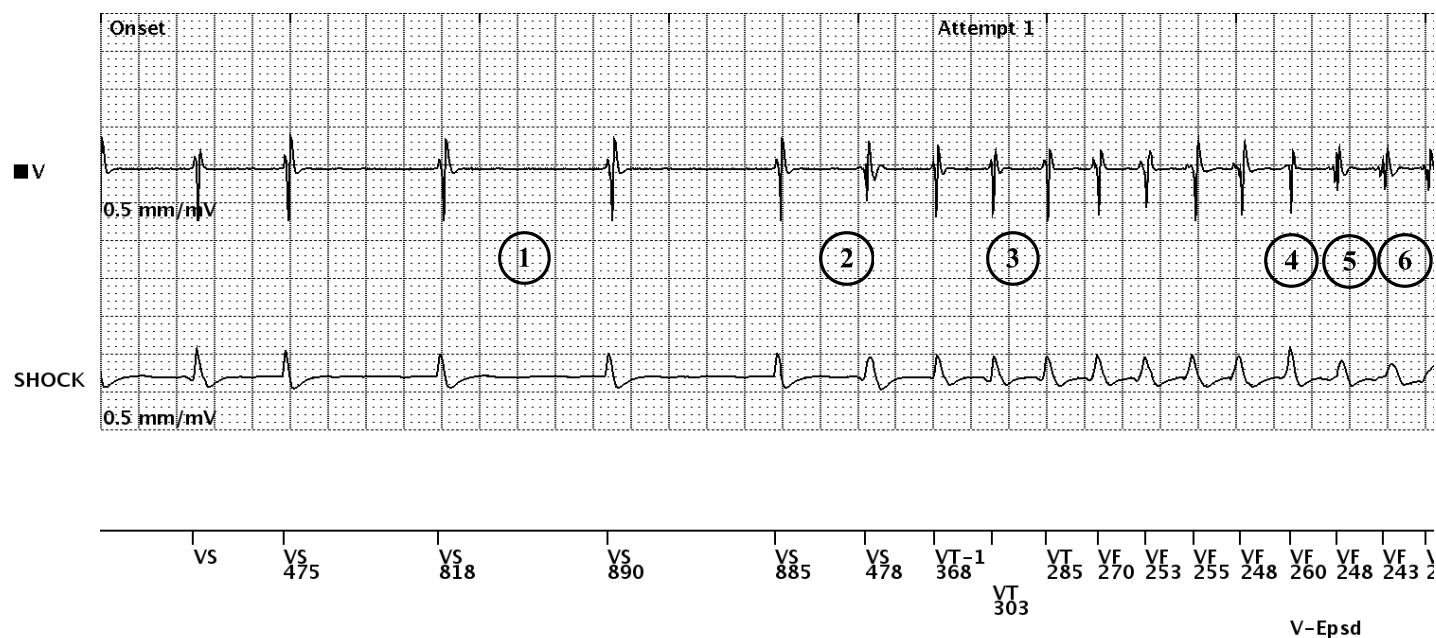

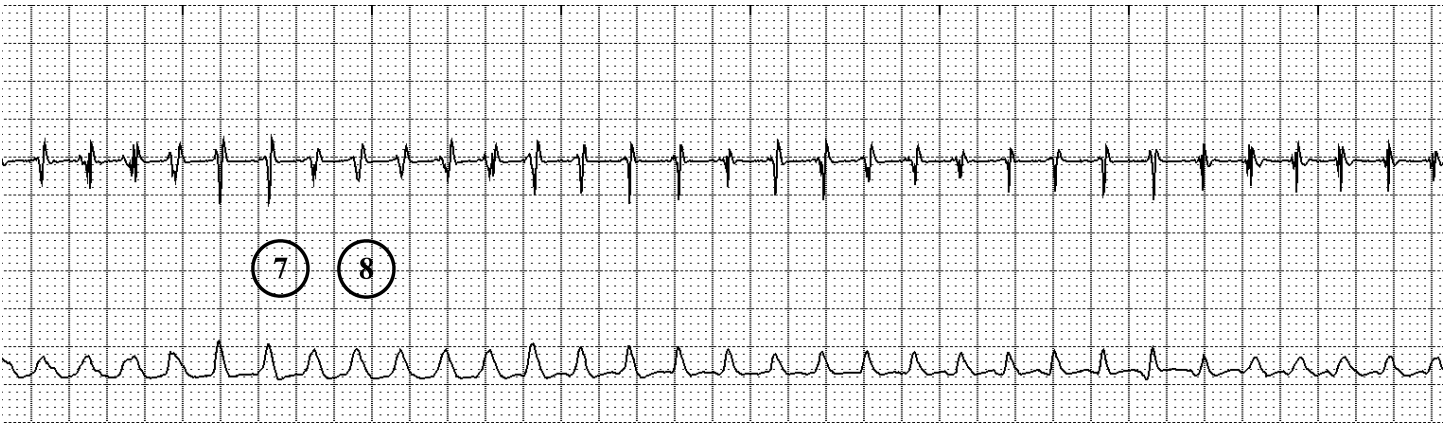

VF 28 VF 243 VF 240 VF 235 VF 233 VF 230 VT 275 VF 235 VF 230 VF 230 VF 240 VF 228 VF 220 VF 263 VF 258 VF 263 VF 260 VF 248 VF 255 VF 245 VF 240 VF 243 VF 248 VF 250 VF 258 VF 263 VF 260 VF 243 VF 248 VF 240 VF 248 2

V-Detect  
Chrg

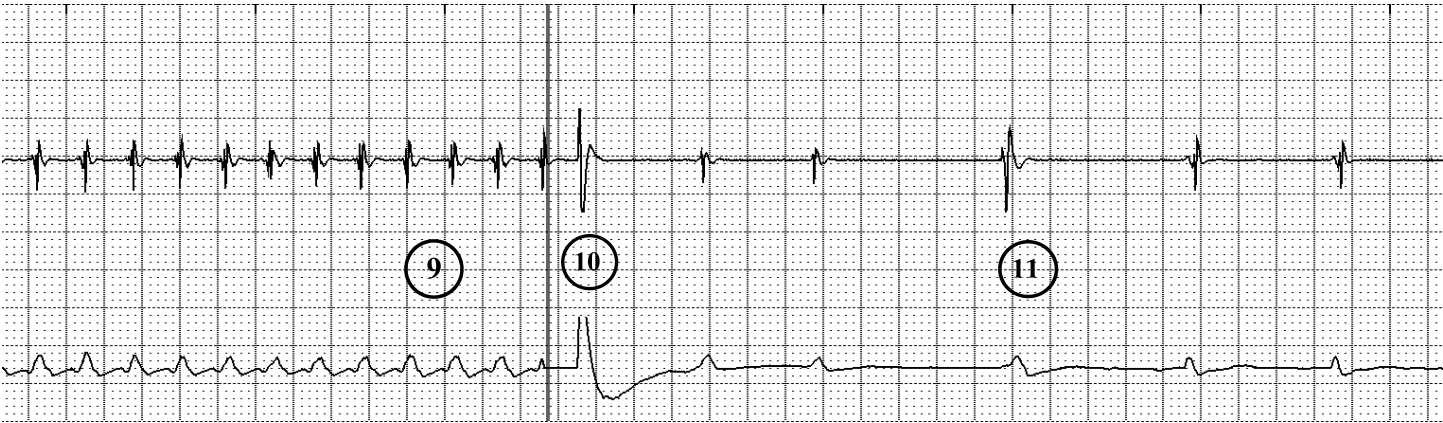

F 40 VF 233 VF 258 VF 253 VF 245 VF 243 VF 233 VF 238 VF 243 [VS] VF 230 VF 243 -- VS 578 VP 1000 VS 980 VS 770

Chrg 41J Shk

